

VETSCAN[®] HM5

Hospital Resource Guide



Welcome

to the VETSCAN® HM5 Hospital Resource Guide

This guide is designed to give you everything you need to get the most out of the VETSCAN HM5 hematology system. Throughout the chapters listed, you will find links to supplemental resources to help address questions.

We hope you find this guide useful. And as always, contact Diagnostic Technical Support for further assistance at:

 (888) 963-8471 (option 5)

 dxsupport@zoetis.com

Need guidance on a treatment plan?

Confirm results and a path forward for complex cases with remote specialist consultations—at no additional charge for Zoetis Diagnostics customers.*

 [ZoetisDx.com](https://zoetisdx.com)

Contents

- > How the VETSCAN HM5 Works
- > Sample Handling
- > Complete Hematology Picture
- > Responsible Patient Trending
- > Histograms
- > Interpretation Guide
- > Alternative Fluids
- > Reference Intervals (Ranges)



How VETSCAN HM5 Works



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

The VETSCAN HM5 is a fully automated, 5-part differential hematology analyzer displaying a comprehensive 22-parameter complete blood count (CBC) with cellular histograms on an easy-to-read touch screen. Its reliable performance, elegant design, ease of use and minimal maintenance with automated reminders make it the optimal veterinary hematology system.

Reliable performance for full CBC analysis



Automated CBC analysis on a wide range of species

- Flexibility to analyze different species
- Ideal for veterinary clinics, including mixed and large animal facilities
 - Five-part differential for 6 species: alpaca, cat, cattle, dog, horse and llama
 - Three-part differential for 9 species: ferret, goat, guinea pig, mouse, pig, primate,* rabbit, rat and sheep



Histograms to complement differentials

- Blood cell populations are graphically represented by cellular histograms
- Can easily verify differential cell counts, help identify uncommon disease processes or check sample integrity at a glance



*For research use only.



How VETSCAN HM5 Works



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids


Reference Intervals (Ranges)

Most automated hematology analyzers used in veterinary medicine are either impedance counters or laser flow cytometers or contain a combination of the two.

The VETSCAN HM5 uses impedance technology for the counting and categorization of cells.


Impedance technology

- In impedance counters, particles (cells) in a blood sample are suspended in an electrolyte solution and passed through an aperture that connects 2 chambers—1 containing a positive electrode and 1 containing a negative electrode
- Passage of a particle through the channel invokes a brief change in the electrical impedance between the electrodes that is proportional to the size of the particle
- Cells pass through the aperture to be classified by voltage emitted
- Measured values from impedance counters include RBC count, MCV, PLT count, WBC count and a 3- to 5-part WBC differential
- From the measured values, additional values—notably MCHC and HCT—are calculated

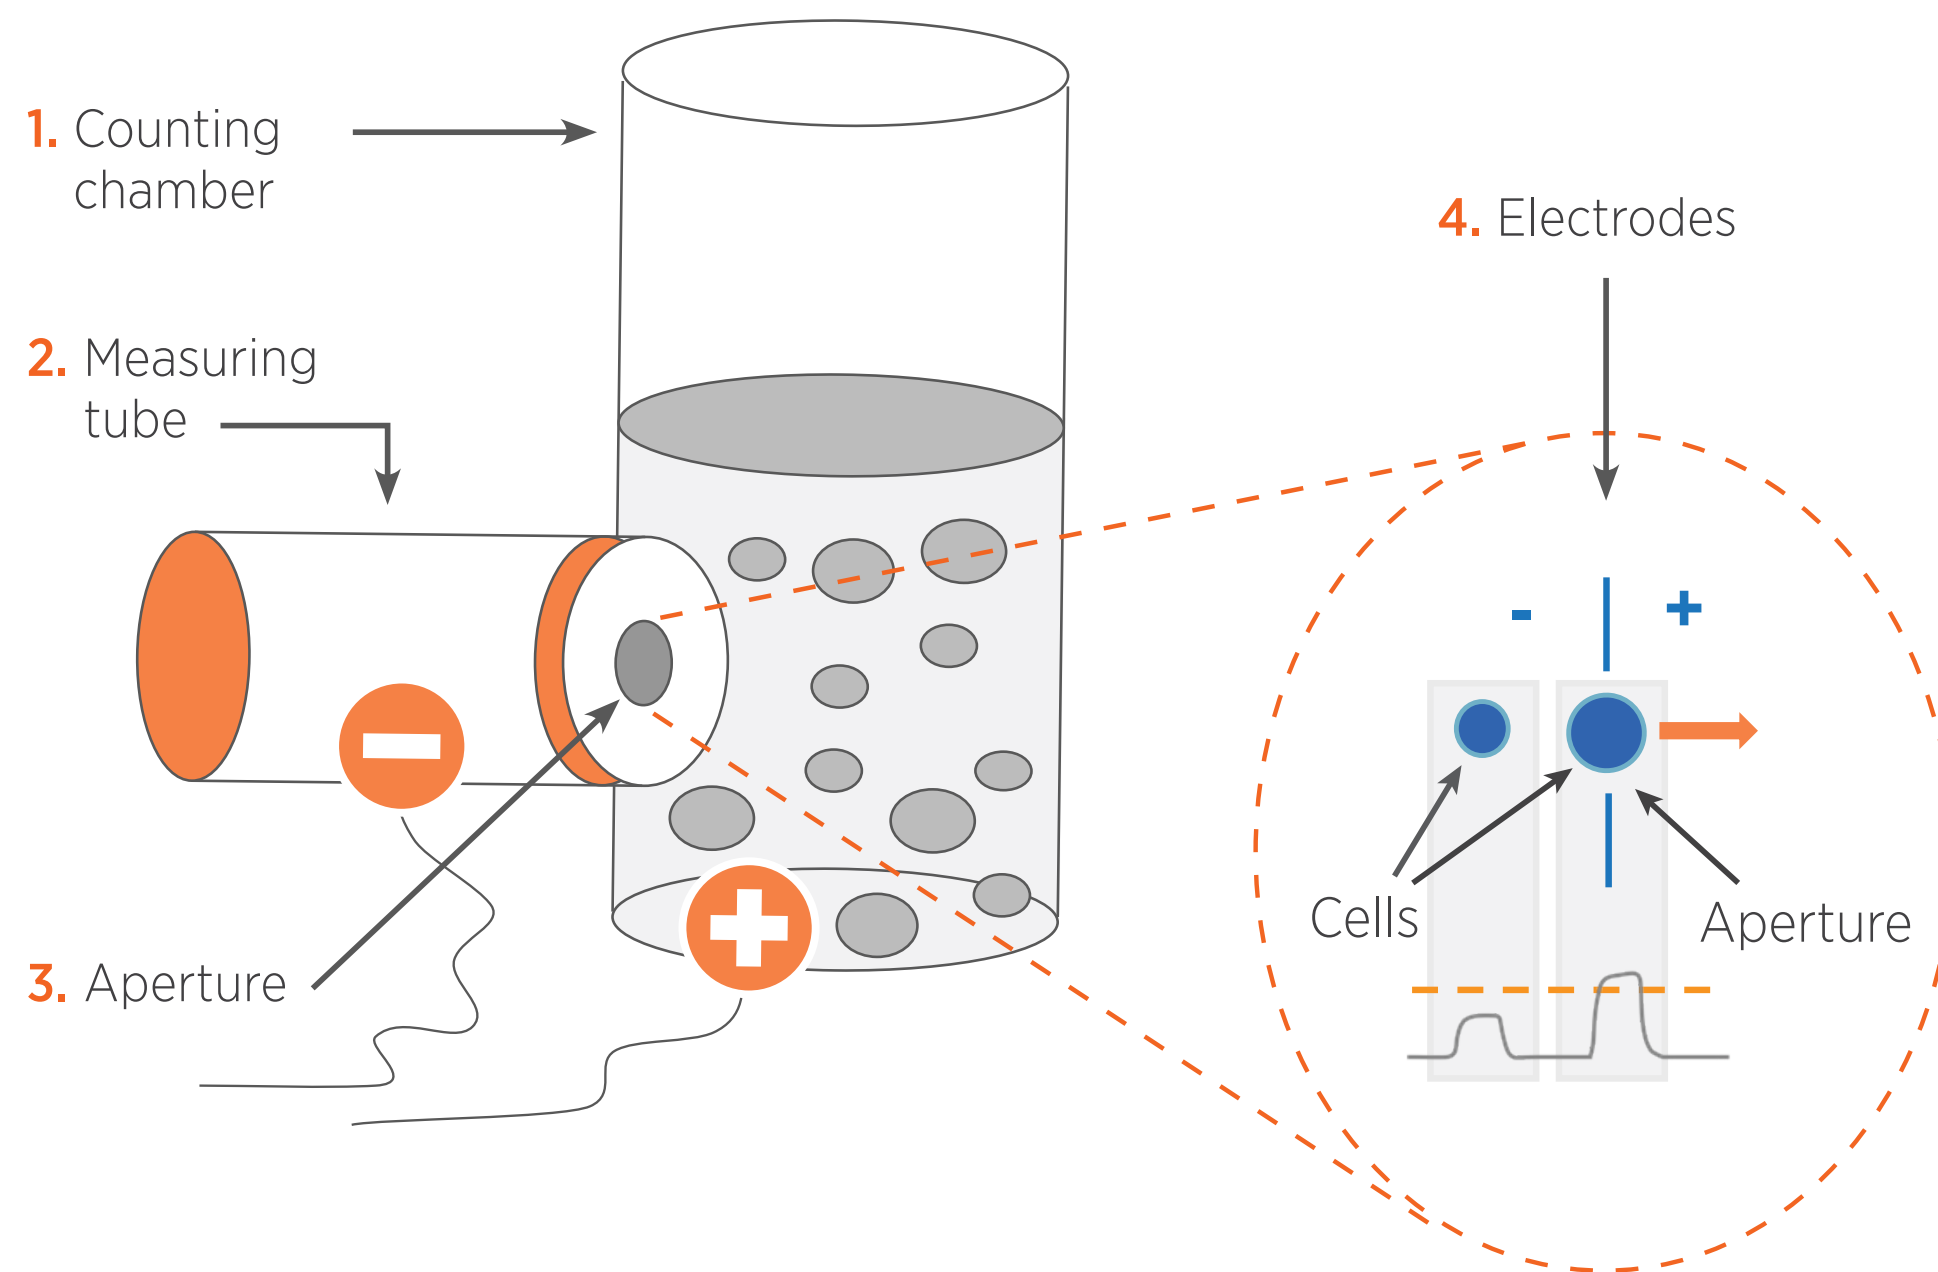

Hemoglobin (HGB) spectrophotometry measurement

- Spectrophotometry measures free HGB (from the lysed RBC and any amount that was already present in the plasma)

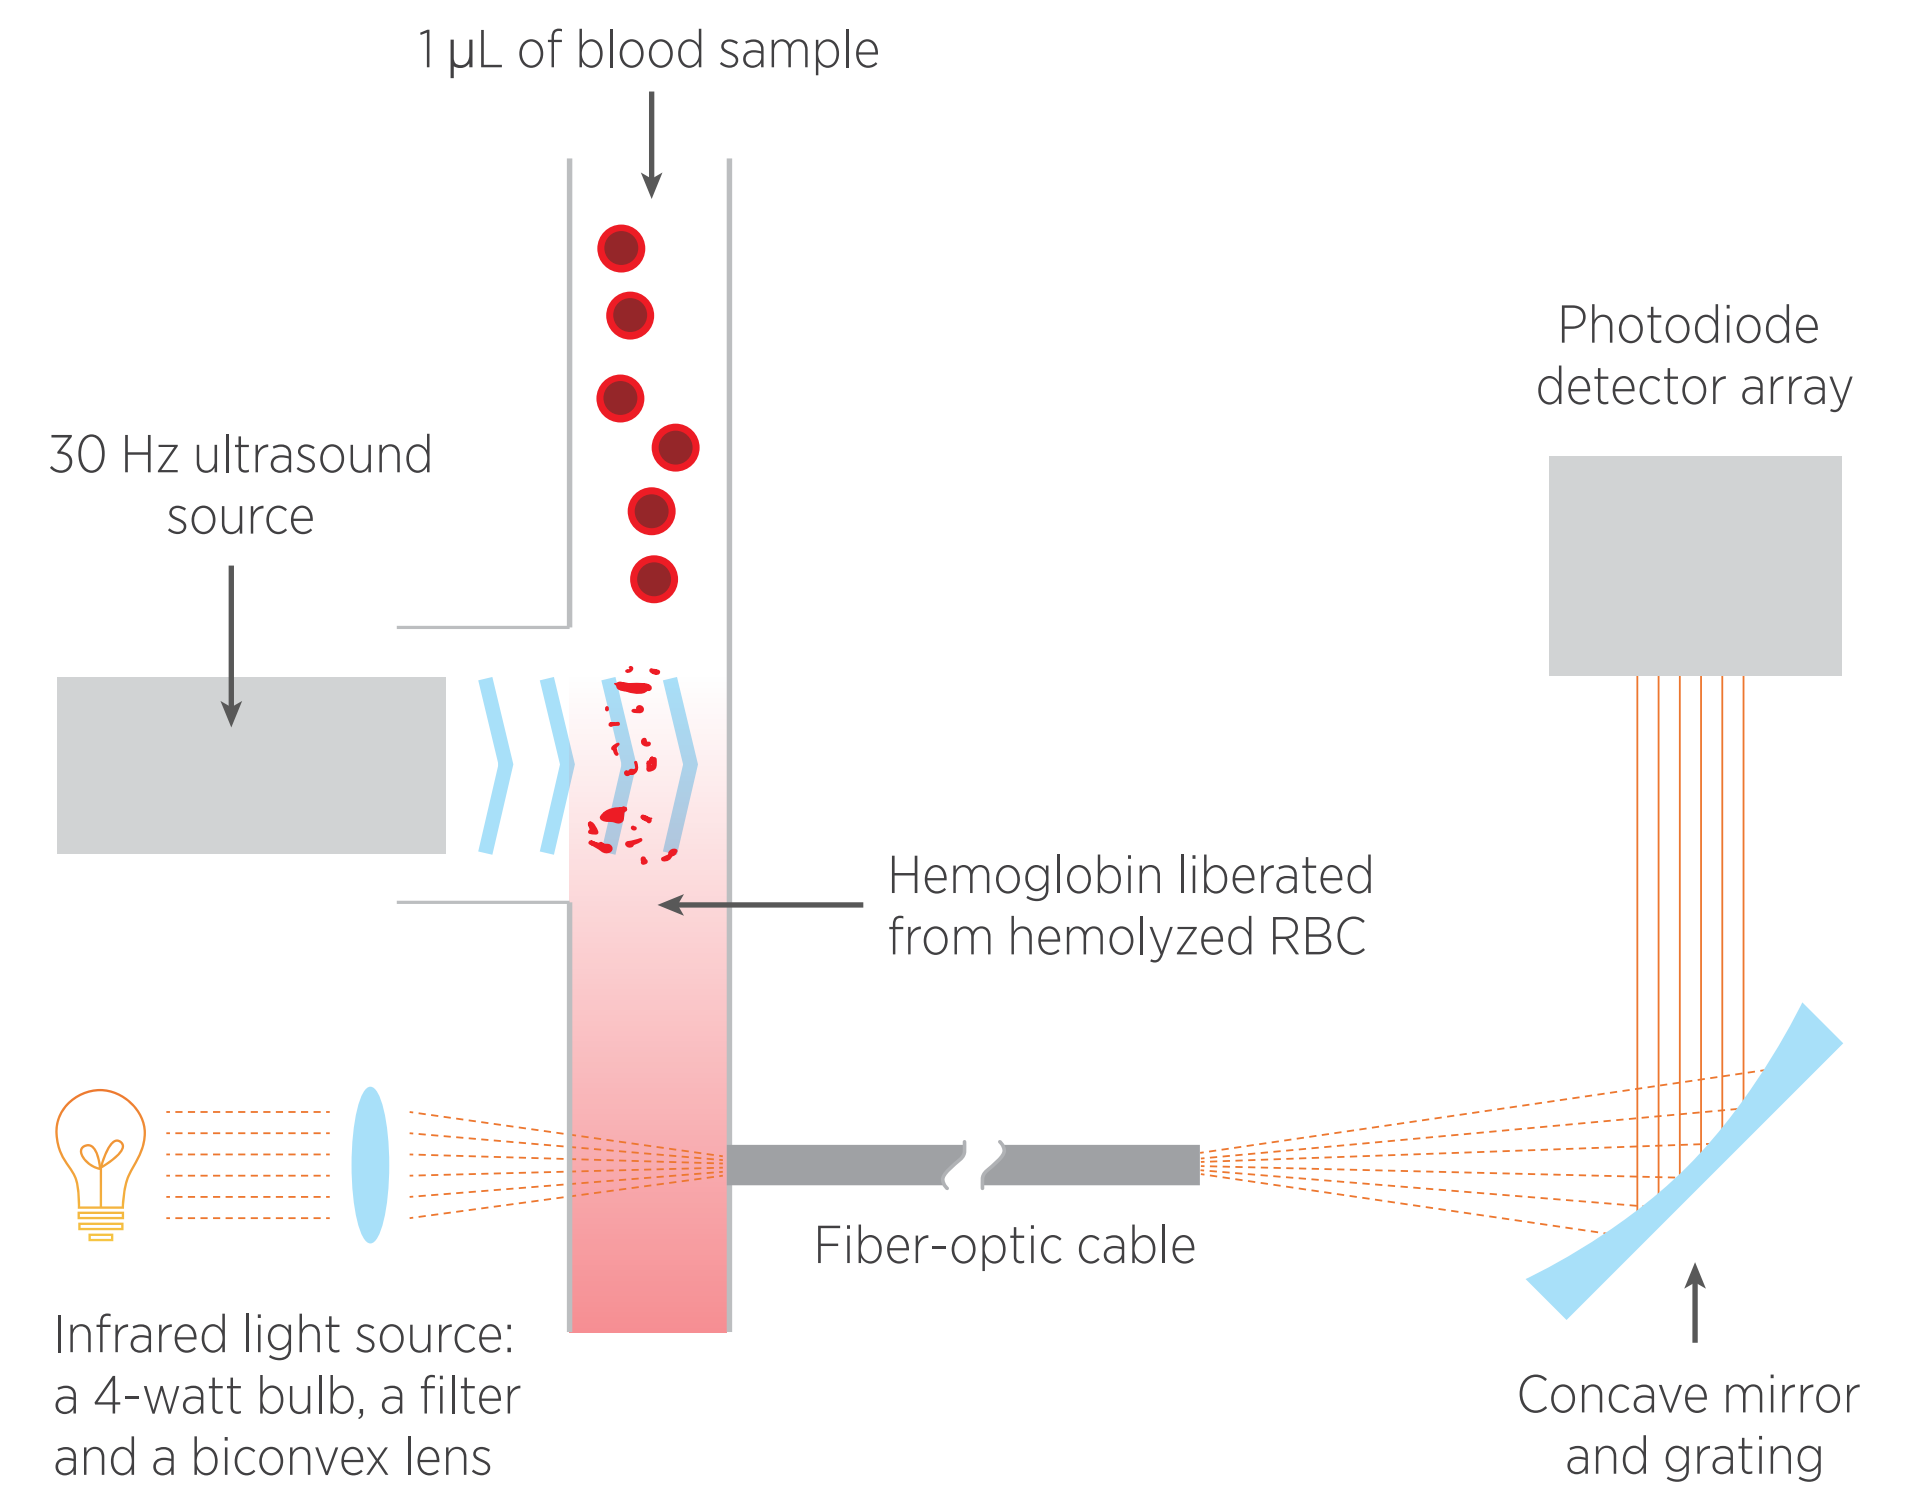

Used with permission from Alex Yartsev.



How VETSCAN HM5 Works



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

VETSCAN HM5 supports 15 species


Species listed here have been validated on the VETSCAN HM5.

- Those not included are not currently supported by Zoetis Diagnostics
- The VETSCAN HM5 cannot be used for avian/reptilian species
- Primate reference intervals are available for research purposes only

The truth behind the 3- and 5-part differential


Automated CBC analyzers are generally classified as either 3-part or 5-part differential analyzers.

5-part differential		3-part differential		
 Dog	 Cat	 Pig	 Goat	 Sheep
 Horse	 Cattle	 Rat	 Ferret	 Mouse
 Alpaca	 Llama	 Guinea Pig	 Rabbit	 Primate*

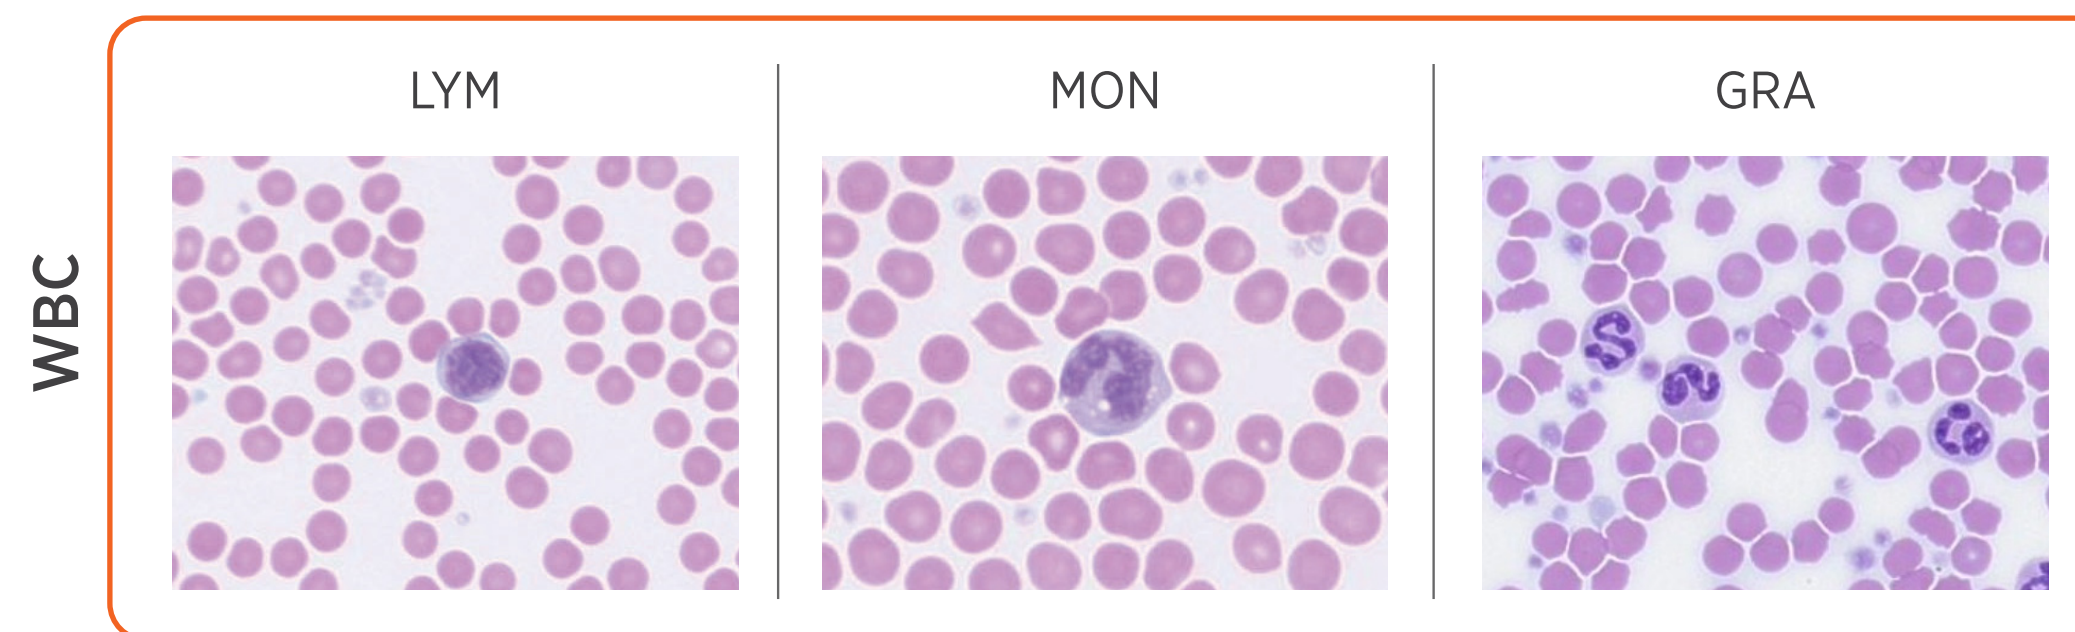

3-Part WBC Differential¹

Images obtained from VETSCAN IMAGYST™.

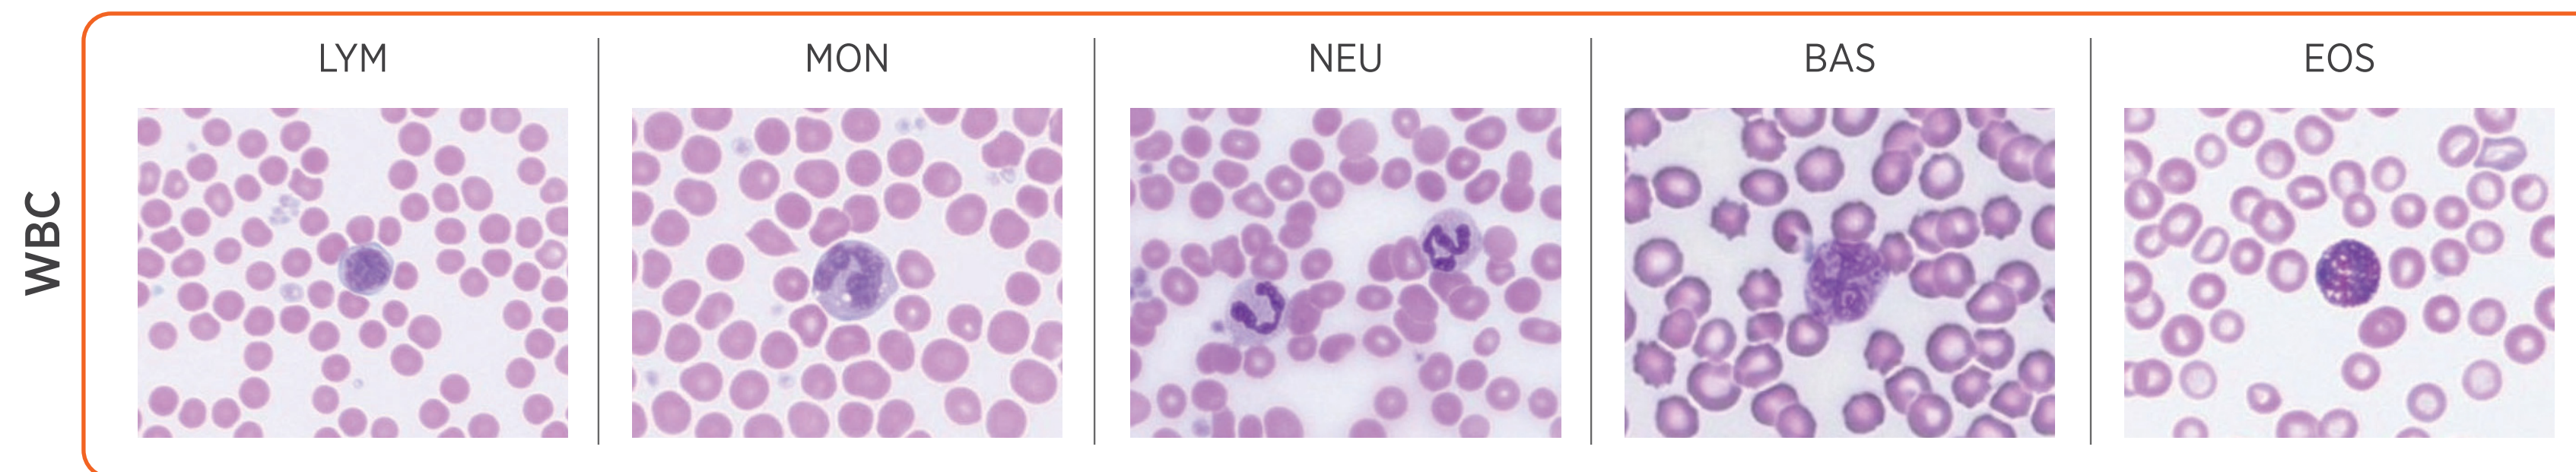

5-Part WBC Differential²

The ability of 5-part differential analyzers to enumerate the less abundant cell types—ie, MON, EOS and BAS—separately, rather than as a mixed cell population, is a significant enhancement.

BAS=basophil; EOS=eosinophil; GRA=granulocyte; LYM=lymphocyte; MON=monocyte; NEU=neutrophil.

*For research purposes only.



Sample Handling



How VETSCAN® HM5 Works

Sample Handling

Patient preparation

Sample collection

Running a sample

Complete Hematology Picture

Minimum database

Automated CBC

Blood smear

PCV/TS

Responsible Patient Trending

Histograms

Interpreting histograms

Histogram examples

Interpretation Guide

Macrothrombocytopenia

Leukogram patterns







Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Patient preparation

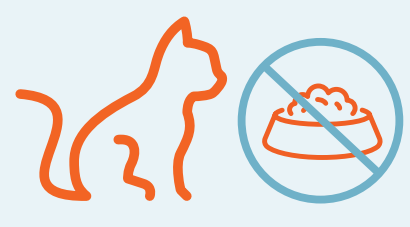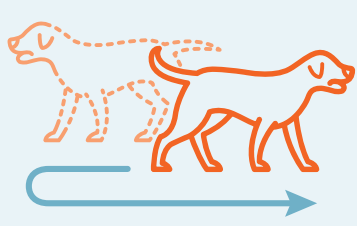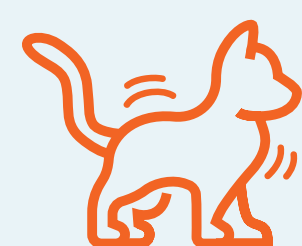These recommendations apply to all laboratories and instruments—whether point-of-care or send-out.

	Before the appointment	Rationale
	<ul style="list-style-type: none"> Avoid feeding patients for 10 to 12 hours prior to appointment unless contraindicated In horses and ruminants, fasting prior to hematology analysis is not required 	<ul style="list-style-type: none"> A postprandial sample may cause lipemic interference Food consumption can cause fluctuations in hematology results—including HGB, MCH and MCHC³
	<ul style="list-style-type: none"> Consider timing of patient appointment relative to when hematologic testing will be completed Understand that certain medications may impact test results 	<ul style="list-style-type: none"> Age-related changes can lead to artifacts in the blood sample for hematology testing—such as RBC crenation, WBC chromatin swelling, platelet clumping⁴ Several chemotherapeutic drugs, NSAIDs and antimicrobial medications are associated with hematologic adverse drug events⁵
	<ul style="list-style-type: none"> Avoid exercise and minimize excitement/fear prior to the appointment 	Can cause: <ul style="list-style-type: none"> Physiological leukocytosis³ Transient hyperglycemia in cats⁶
	At the clinic	Rationale
	<ul style="list-style-type: none"> Minimize excitement/fear during the appointment Consider the use of sedation and antianxiety medications to help decrease stress for anxious animals and enable safer and gentler restraint, when appropriate 	Can cause: <ul style="list-style-type: none"> Physiological leukocytosis³ Transient hyperglycemia in cats⁶
	<ul style="list-style-type: none"> With a sick patient, anticipate that analyte results may be impacted 	<ul style="list-style-type: none"> Visually inspect for clots that can falsely impact cell counts and harm the analyzer Visual assessment of the sample preanalysis can highlight abnormalities (eg, hemolysis can indicate poor sample quality) or may indicate the presence of disease
	At time of sampling	Rationale
	<ul style="list-style-type: none"> Good sample collection technique is critical (clean needle puncture of the vein, etc) 	<ul style="list-style-type: none"> Lack of good technique leads to an increased risk of clotted sample or hemolysis

MCH=mean corpuscular hemoglobin; NSAID=nonsteroidal anti-inflammatory drug.

[Get more sample handling best practices ↗](#)



Sample Handling



How VETSCAN® HM5 Works

Sample Handling

Patient preparation

Sample collection

Running a sample

Complete Hematology Picture

Minimum database

Automated CBC

Blood smear

PCV/TS

Responsible Patient Trending

Histograms

Interpreting histograms

Histogram examples

Interpretation Guide

Macrothrombocytopenia

Leukogram patterns

Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Keys to successful sample collection

The quality of the sample analyzed is directly related to the quality of the result.

<p>Avoid vein collapse when drawing samples</p>	<ul style="list-style-type: none"> Minimize suction on the syringe, and do not draw back too quickly
<p>Prevent hemolysis</p>	<ul style="list-style-type: none"> Use the largest vein and needle appropriate for blood collection Avoid use of any needle smaller than a 23 gauge (though certain exotic species may require a smaller needle) Use minimal alcohol on fur/skin Remove the needle from the syringe before dispensing into the blood tube unless using a closed vacuum blood collection system
<p>Ensure the correct ratio of anticoagulant to blood</p>	<ul style="list-style-type: none"> Fill EDTA tube to manufacturer's sample fill line Immediately after filling tube, cap the tube and invert 10-15 times to sufficiently mix with anticoagulant (more inversions would be needed in case of 0.25 mL, 0.5 mL or 1.3 mL tubes)
<p>Ensure appropriate tube use</p>	<ul style="list-style-type: none"> Select tubes based on the testing requirements and size of patient (Microtainer®, 1.3 mL, 3 mL, 5 mL) Ensure tubes have not expired Always fill blood tubes in the correct order to avoid contamination <ul style="list-style-type: none"> EDTA contamination of chemistry samples may affect electrolyte results and cause a falsely low Ca and falsely high K⁺ If improper tube-filling order occurs, the sample should be redrawn <div data-bbox="1153 1401 2710 1660"> <p>Blood tube fill order</p> <p>1 SODIUM CITRATE anticoagulant for coagulation testing → 2 NO ANTICOAGULANT for chemistry → 3 LITHIUM HEPARIN anticoagulant for chemistry → 4 EDTA anticoagulant for hematology</p> </div>
<p>Prevent unwanted blood clotting</p>	<ul style="list-style-type: none"> Do not hold off the vein for more than a few seconds before venipuncture For feline samples collected from the medial saphenous vein, a vacuum blood collection system instead of a syringe is recommended
<p>Do not allow samples to degrade</p>	<ul style="list-style-type: none"> Run samples as soon as possible after drawing

Ca=calcium; EDTA=ethylenediaminetetraacetic acid; K⁺=potassium.



Sample Handling



How VETSCAN® HM5 Works

Sample Handling

Patient preparation

Sample collection

Running a sample

Complete Hematology Picture

Minimum database

Automated CBC

Blood smear

PCV/TS

Responsible Patient Trending

Histograms

Interpreting histograms

Histogram examples

Interpretation Guide

Macrothrombocytopenia

Leukogram patterns

Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Running a sample on the VETSCAN HM5⁷

DO's

- Always use an EDTA collection tube—no other tubes are validated
- Always fill the collection tube to the manufacturer's sample fill line
- Test as soon as possible after sample collection
- Refrigerate if it will be >20 minutes until sample can be run to preserve cell morphology
 - Allow sample to warm to room temperature prior to running on the VETSCAN HM5
- Reinvert the tube 10 to 15 times after the sample is collected AND again just prior to running on the VETSCAN HM5
- Create a blood smear shortly after collection—no need to stain or evaluate slide right away
- Check for blood clots before running the sample
- Select the correct species to be analyzed, as the algorithms and cell sizes differ by species
 - If the original species selected was incorrect (eg, if a canine sample was run as a feline), rerun the sample under the correct species

DON'Ts

- Freeze sample
- Use if tube not filled to manufacturer's sample fill line—an incorrect ratio of EDTA to blood can affect results
- Run a sample with a visible blood clot
- Run a sample straight from the refrigerator without warming to room temperature

Spurious errors^{8,9}

Keep in mind that anything that spuriously affects RBC or MCV will in turn spuriously affect MCHC and HCT. Anything that spuriously affects HGB will also affect MCHC. Inaccurate results are possible if the analyzer is out of calibration.

Spurious results/errors	Cause	Prevention: Always include a blood smear to help with interpretation
↑ HGB	Hemolysis, lipemia, icterus, Heinz bodies, severe leukocytosis	Prevent hemolysis and lipemia
↑ MCV	Prolonged storage at room temperature, RBC swelling, autoagglutination, some regenerative anemia cases	Run sample immediately or store in refrigerator
↑ MCHC	Hemolysis, lipemia, many Heinz bodies, storage at room temperature or false increase in HGB, marked spherocytosis	Most of these causes can be prevented with proper sample handling techniques
↓ PLT	PLT clumping, blood clots, macroplatelets	Prevent through proper sample handling, needle size and vein selection. Fill tube to manufacturer's sample fill line and invert tube immediately after collection and just prior to running on analyzer
↑ RBC	Dehydration, macroplatelets	Consider patient health status and breed variations
↓ RBC	Blood clots, agglutination	Use proper sample handling to avoid blood clots. Never run a clotted sample

Complete Hematology Picture



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

Minimum database

- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples


Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Define your laboratory testing minimum database¹⁰

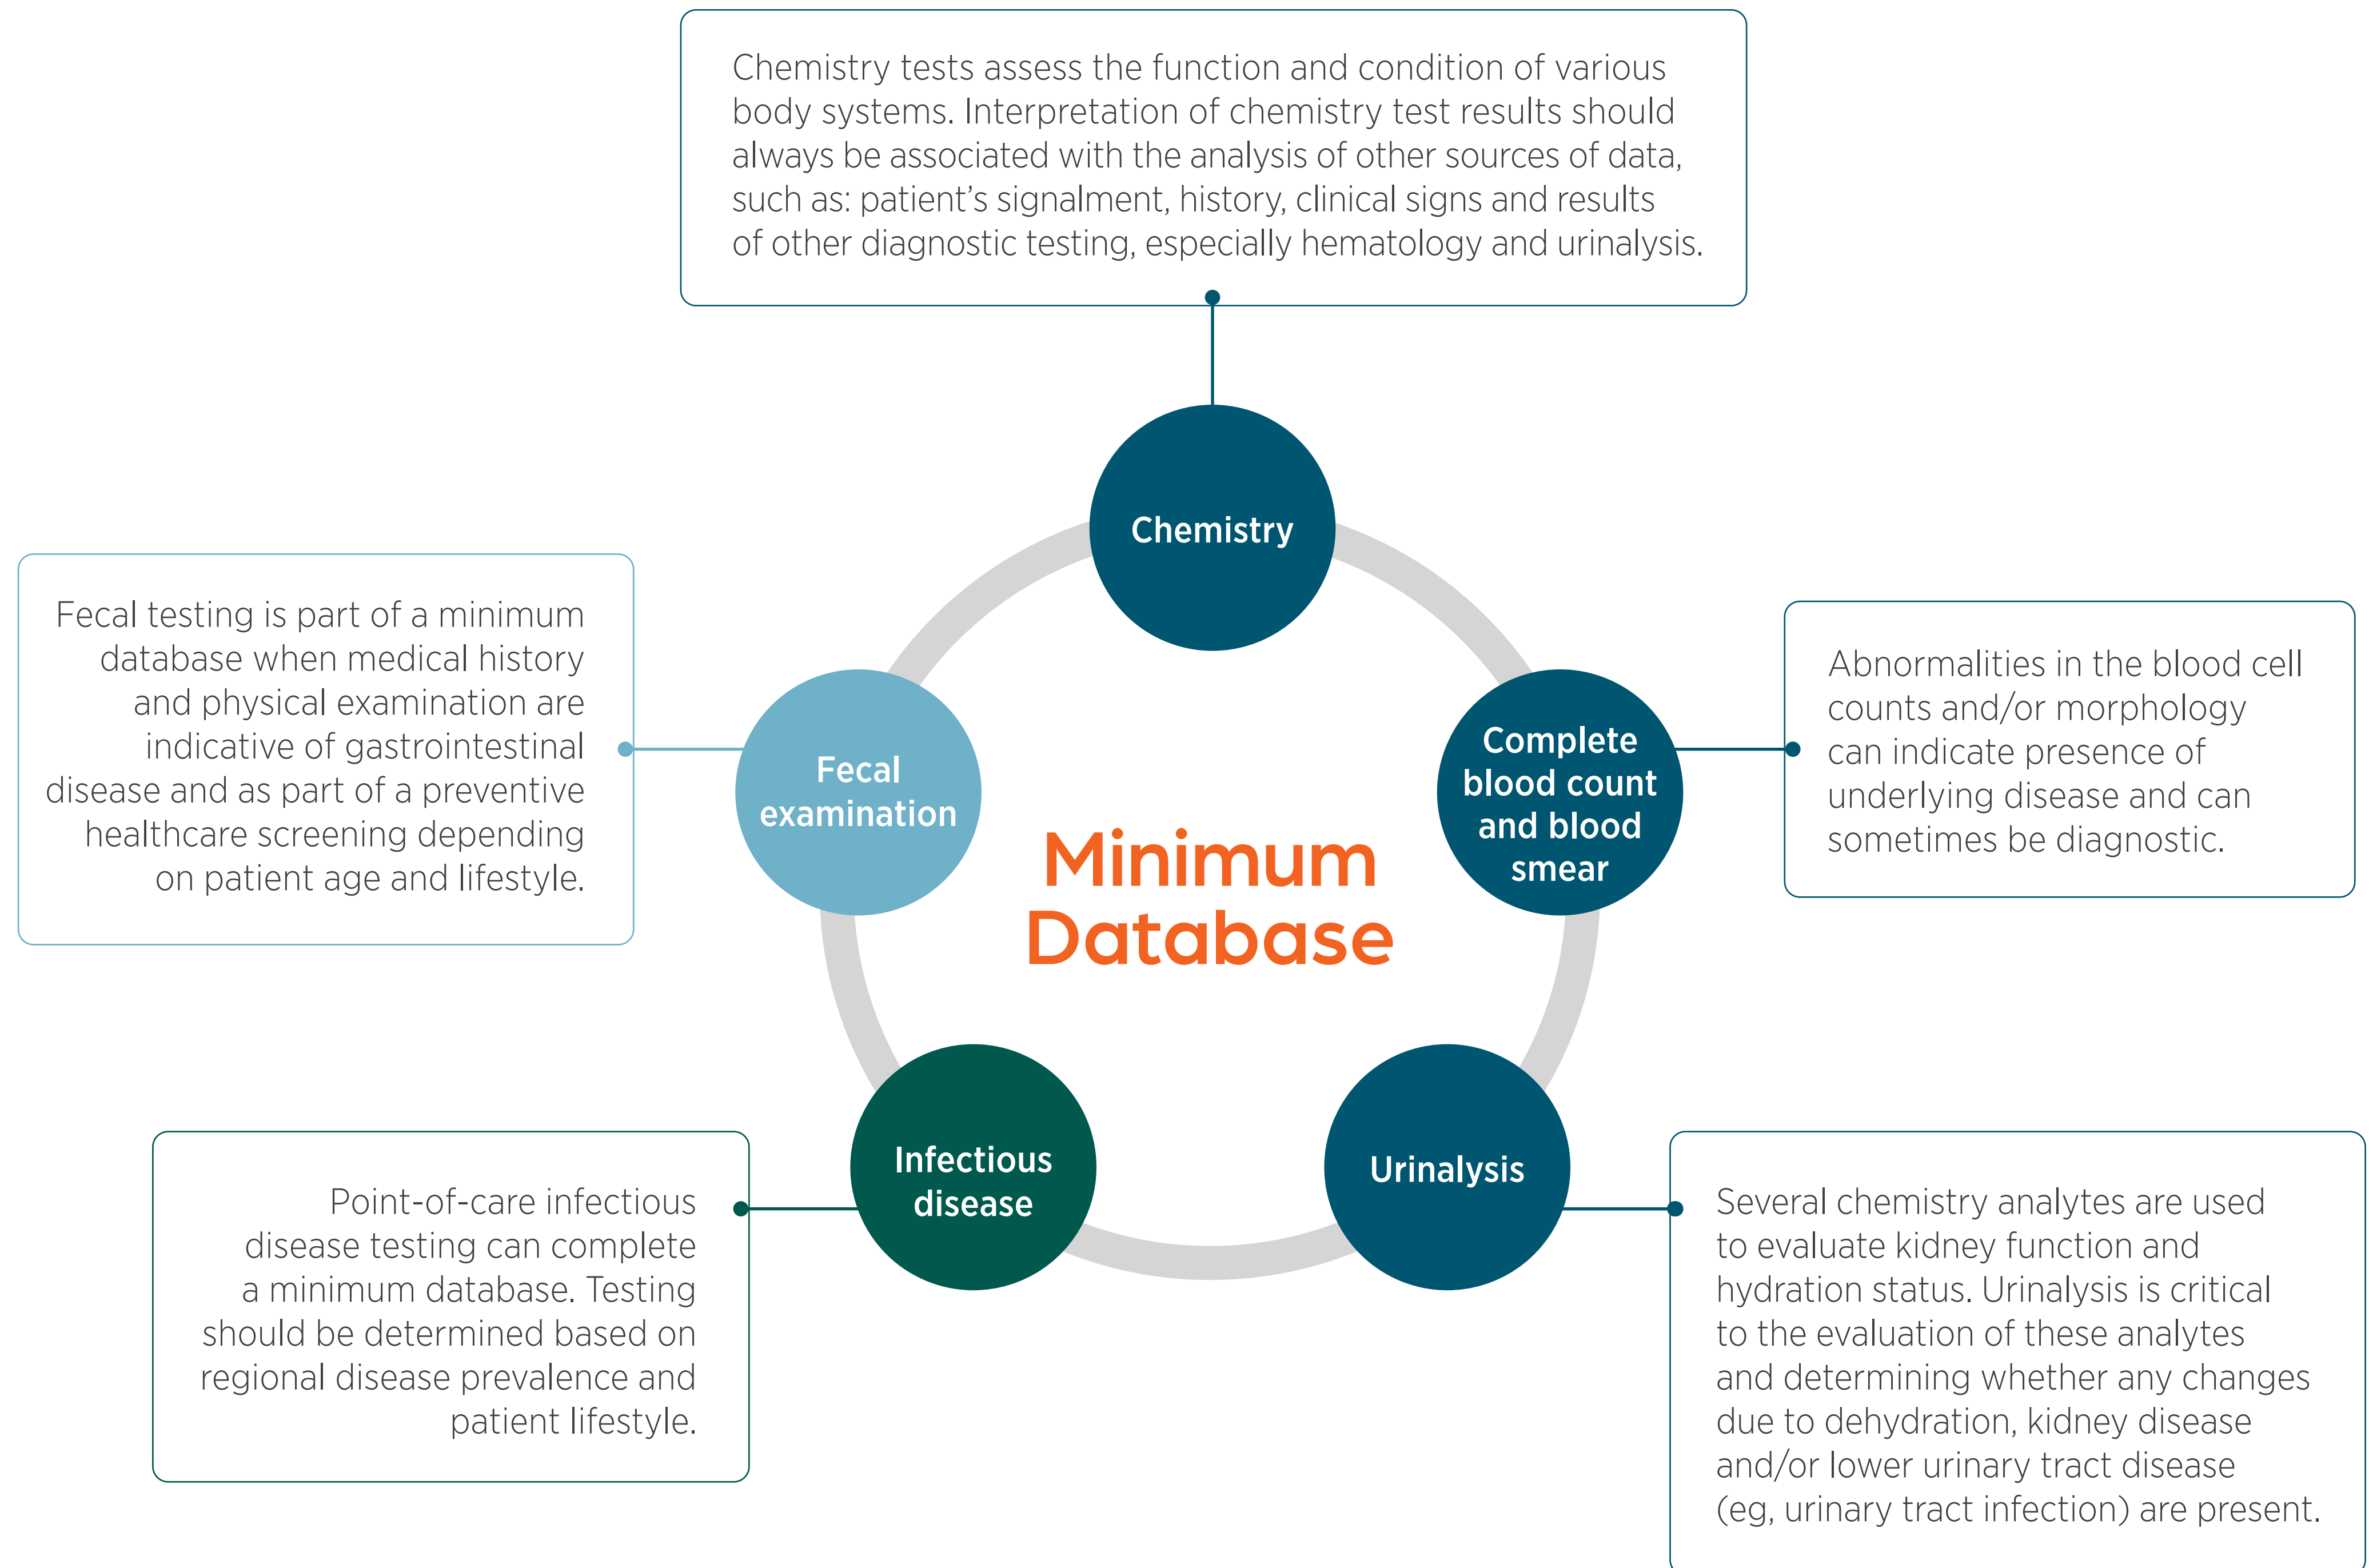

Complete Hematology Picture



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

A complete hematologic picture includes the following CBC components:

- 1 Automated CBC (quantitative)
- 2 Blood smear (qualitative) Manual or using artificial intelligence (AI)
- 3 Packed cell volume (PCV)

Quantitative evaluation: automated CBC

The automated CBC is a diagnostic tool that classifies, enumerates and differentiates the different types of cells present in the peripheral blood. This **quantitative** evaluation of the blood provides different cell population counts and their associated indexes as well as graphic representations when performed on an automated analyzer.

An automated CBC also includes a differential WBC count, which is a breakdown of the amount of each subpopulation of the WBC present in the total WBC population.

Since each WBC has a very specific function, the differential count may be used to identify abnormal levels of specific WBC subpopulations and may offer diagnostic information about specific underlying health conditions.

[Learn more about histograms](#) ↗

ZoetisDx


Clinic Name : Zoetis Demo Hospital
Requesting Doctor : Dr. Smith

Owner Name : Jenna Jones
Patient Name : Luna
Patient ID : 12345

Species : Canine
Breed : N/A

Hematology

Test	Ref Range	Units	Graph	08/27/21 19:17	10/04/22 16:02
WBC	6 - 17	10 ⁹ /l		13.79	13.93
LYM	1 - 4.8	10 ⁹ /l		2.76	2.48
MON	0.2 - 1.5	10 ⁹ /l		0.73	1.13
NEU	3 - 12	10 ⁹ /l		10.03	10.14
EOS	0 - 0.8	10 ⁹ /l		0.19	0.14
BAS	0 - 0.4	10 ⁹ /l		0.07	0.04
LYM%		%		20.0	17.8
MON%		%		5.3	8.1
NEU%		%		72.8	72.8
EOS%		%		1.4	1.0
BAS%		%		0.5	0.3
RBC	5.5 - 8.5	10 ¹² /l		8.11	7.48
HGB	12 - 18	g/dl		16.8	15.6
HCT	37 - 55	%		52.56	53.71
MCV	60 - 77	fl		65	72
MCH	19.5 - 24.5	pg		20.7	20.9
MCHC	31 - 39	g/dl		32.0	29.1
RDWc	14 - 20	%		17.5	16.4
RDWs		fl		40.6	43.0
PLT	165 - 500	10 ⁹ /l		297	248
MPV	3.9 - 11.1	fl		11.0	10.3
PCT		%		0.33	0.25
PDWc		%		40.0	40.0
PDWs		fl		17.9	17.9

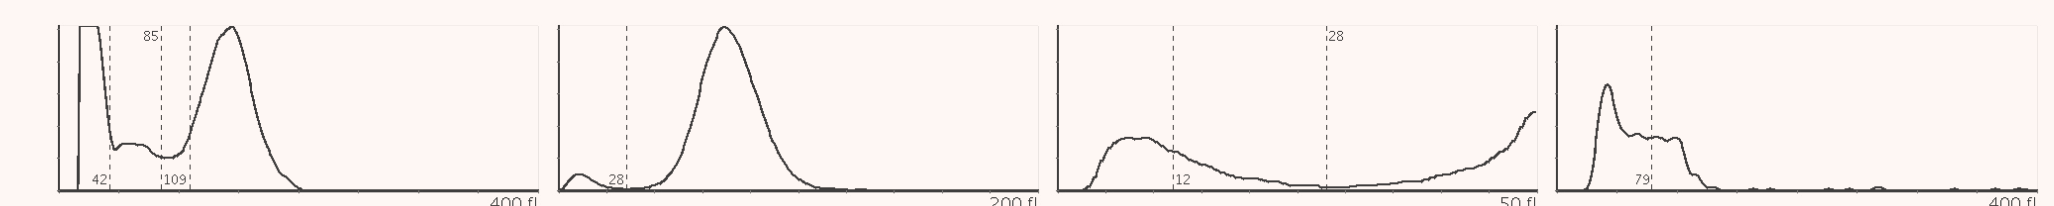



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)


Qualitative evaluation: blood smear

A blood smear is a **qualitative** part of the comprehensive CBC that is used to confirm results, assure quality, and may provide additional insights to guide diagnosis and treatment.¹¹⁻¹⁴ Microscopic examination of a blood smear is an essential part of the hematologic picture, as it can provide vital diagnostic information that is not identified on the automated CBC.

Ideally, a blood smear evaluation should always be performed with every CBC, but it is vital that one be performed in the following clinical instances⁸:

- Anemia (low RBC count)
- Thrombocytopenia (low PLT count)
- Neutrophilia or neutropenia (verify count and examine cells)
- Lymphocytosis
- Severe illness (eg, sepsis)
- Suspicion of parasites
- When certain warning flags are present on the automated CBC report

A blood smear evaluation should not be utilized as a replacement for an automated CBC, as automated analyzers count thousands of cells for more precise and accurate data than manual cell counting. Machines must be properly maintained for consistent precision and accuracy.¹⁵

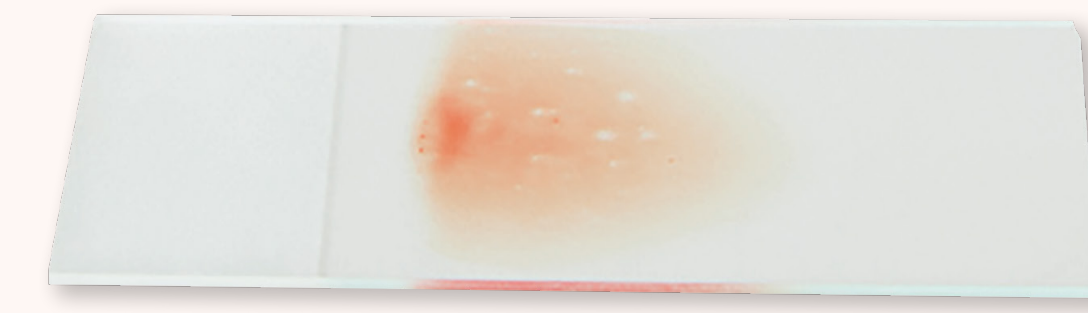

A **blood smear** enables the veterinarian to confirm results and assure quality and may provide additional insights to guide diagnosis and treatment.¹¹⁻¹⁴

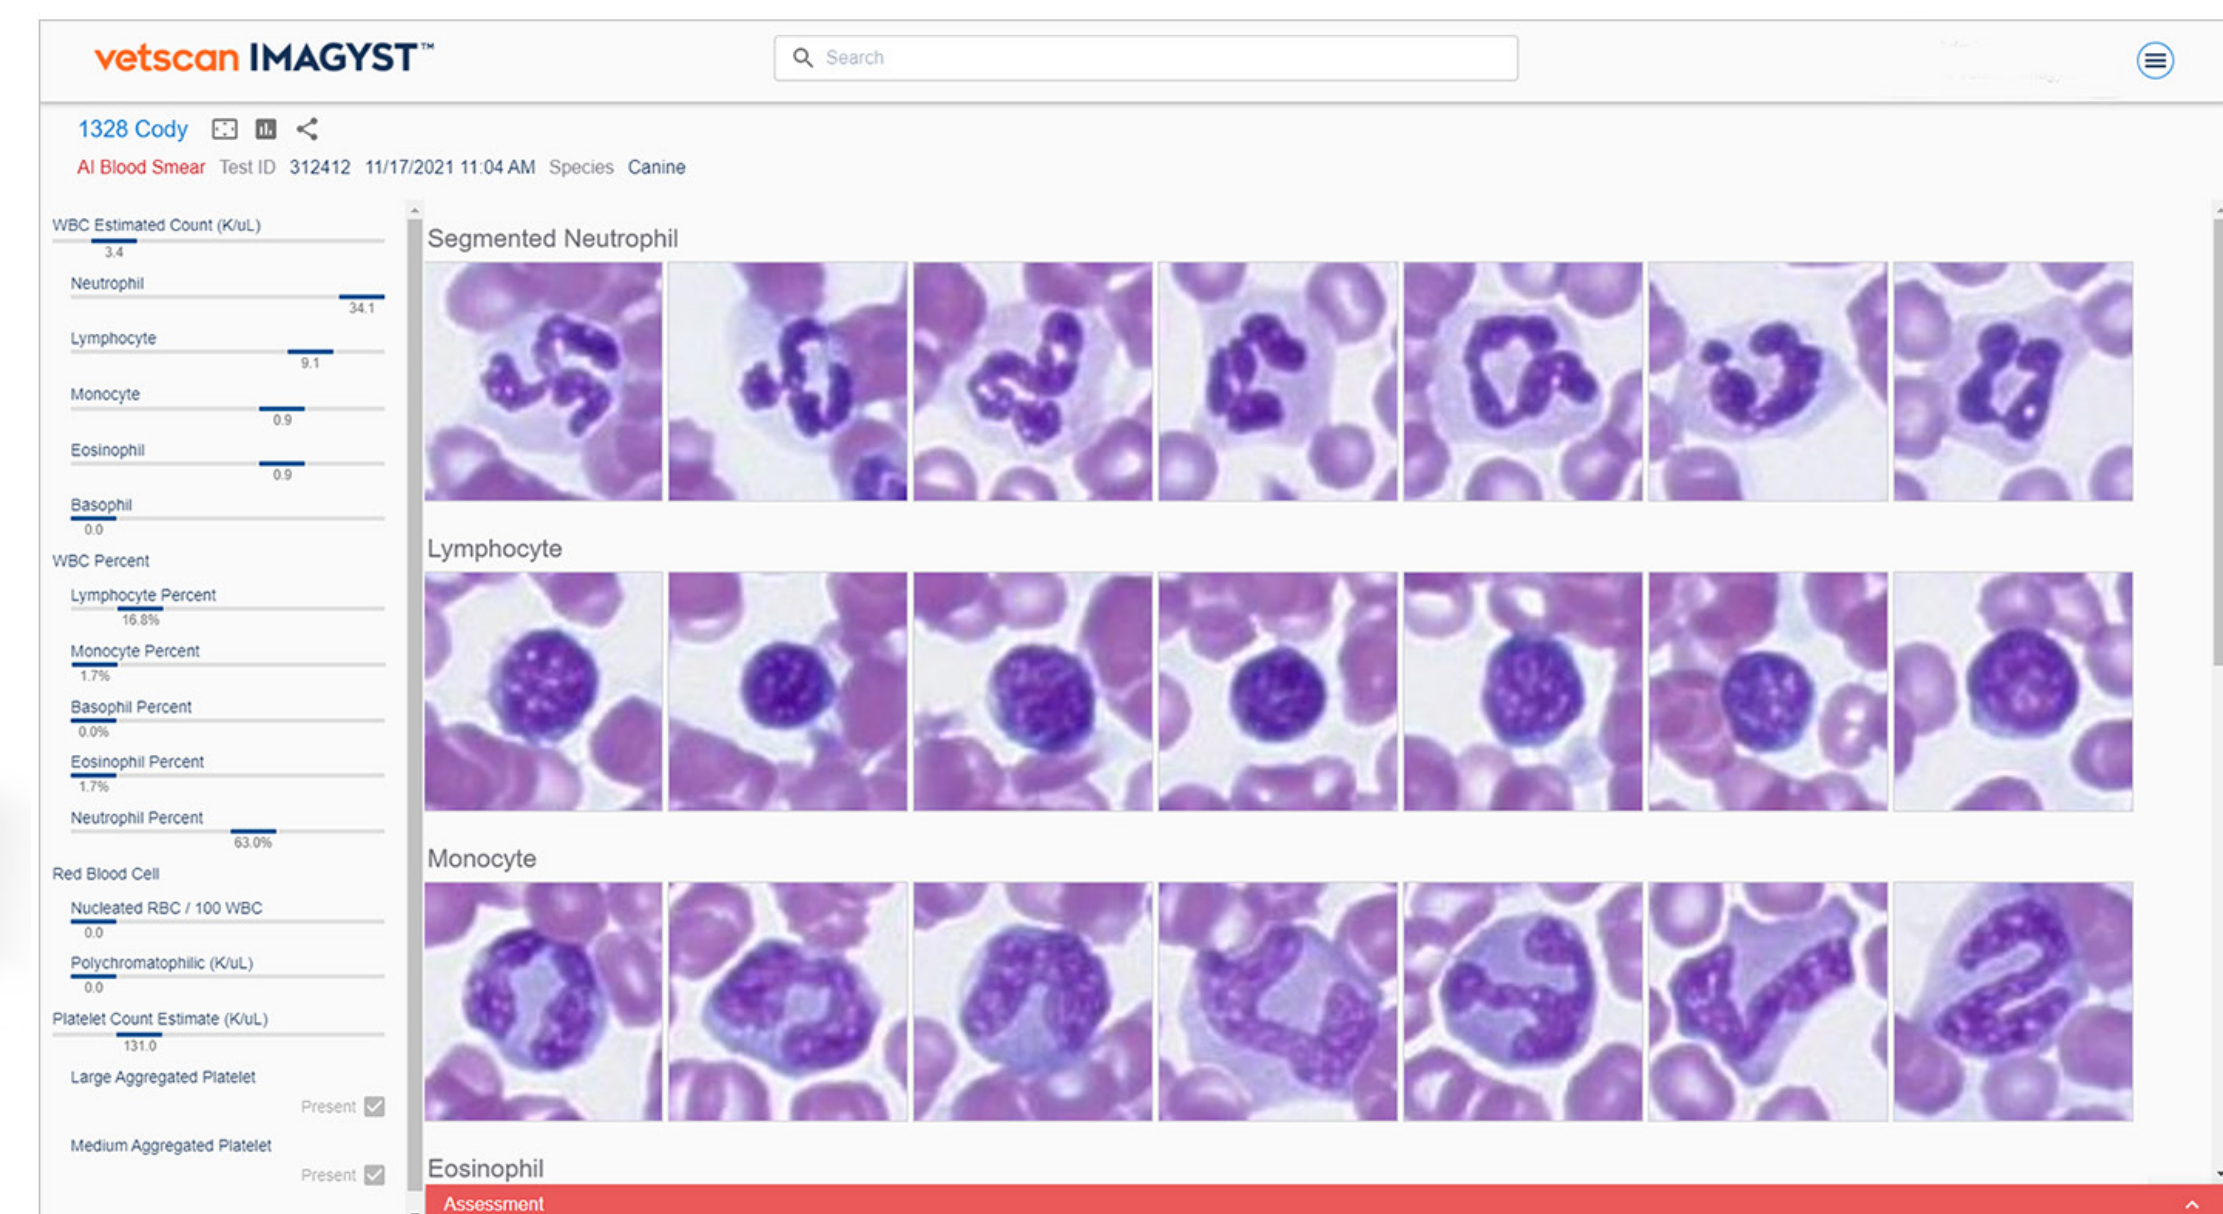


Figure: VETSCAN IMAGYST™ AI Blood Smear sample report

Complete Hematology Picture



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Further quantitative evaluation: PCV/TS


PCV is the direct centrifugal measurement of the percentage of the blood that consists of RBC. It is an accurate measurement with minimal inherent error (+/- 1%).¹⁶

HCT is a calculated value of the percentage of the blood that consists of RBC: $HCT (\%) = (RBC/\mu L) \times MCV (fL/10)$.¹⁷ Unlike PCV, the potential for error is greater with the HCT method because it is subject to MCV variation that can occur with certain hematologic conditions (eg, agglutination) and/or improper sample handling (eg, excess EDTA, hemolysis or inadequate mixing).¹⁸

To verify that HCT was not affected by artifactual errors, perform a PCV measurement¹⁹

HCT (%) can also be estimated with this calculation, using the HGB result from the automated CBC report:

$$HGB \times 3 \text{ (SI units: } HGB \times 0.3)$$

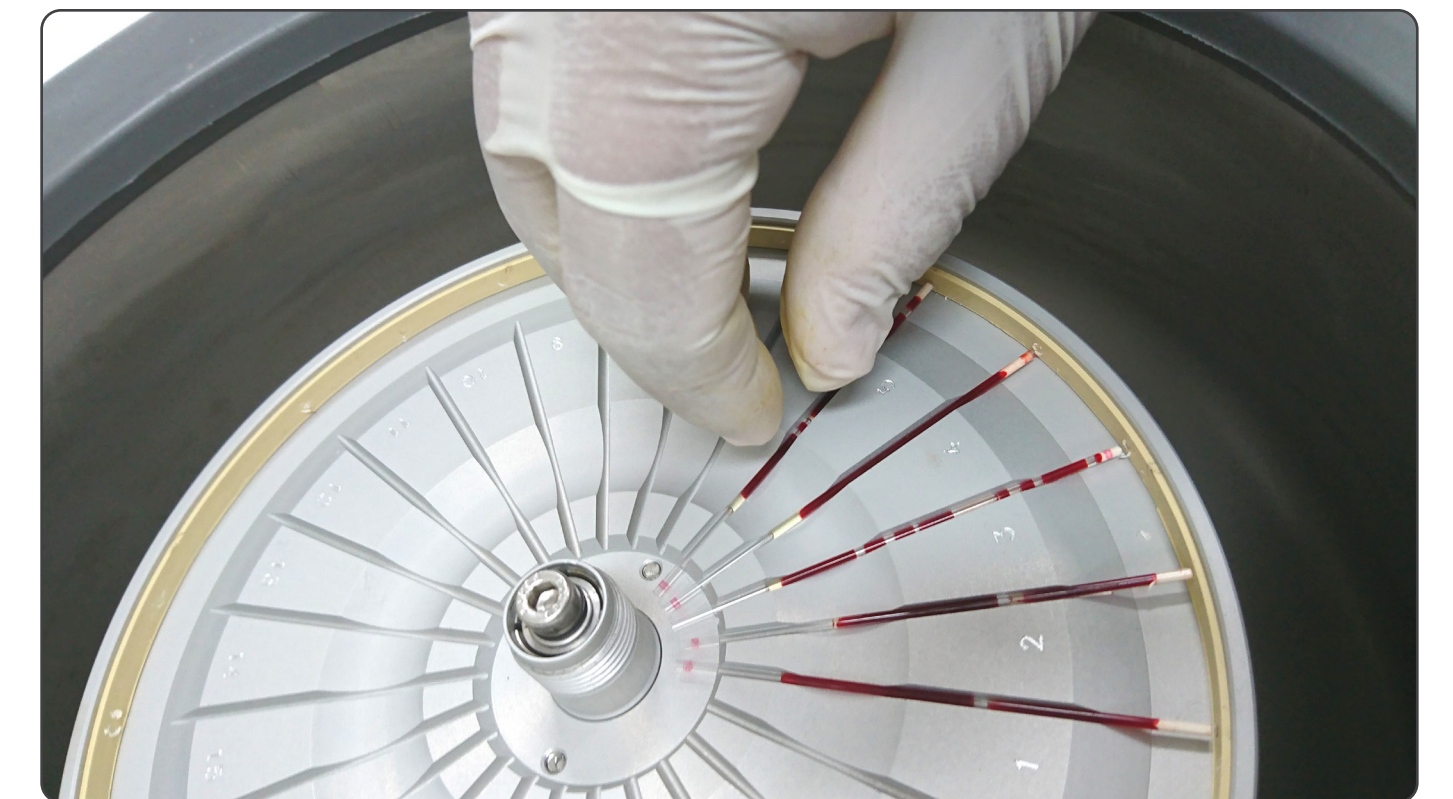

Zoetis Diagnostics delivers a complete hematology solution

A streamlined workflow makes it easy to get to the harder diagnoses




Start with VETSCAN HM5 for quantitative CBC results



Always supplement automated CBC with qualitative results from VETSCAN IMAGYST™ AI Blood Smear



Add on clinical pathologist review when needed*

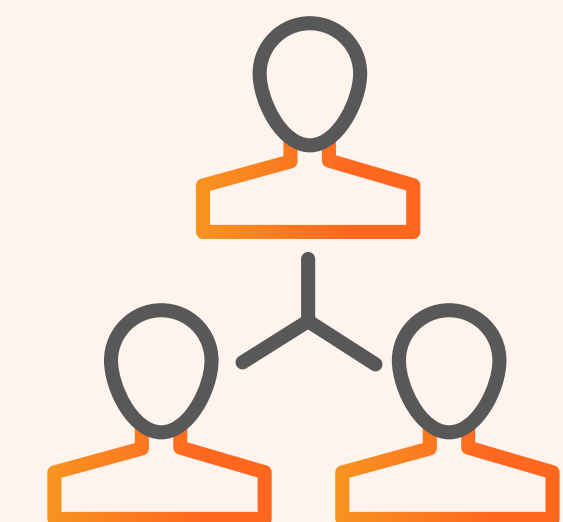

Consult veterinary specialists for challenging cases directly through [ZoetisDx†](#)

AI=artificial intelligence; HCT=hematocrit; MCV=mean cell volume; PCV=packed cell volume; TS=total solids.

*If abnormalities are observed, expert review via digital image transfer is available. This can be done within the VETSCAN IMAGYST system. Additional costs may apply.

†Available in select markets.



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Responsible Patient Trending—why perform?

Due to biological variations, the best reference values are a pet's own diagnostic values over time, encompassing breed, age, sex and individual variation

- Most reference intervals represent results expected for 95% (19 of 20) of a healthy population, and therefore 1 of 20 healthy animals is expected to have a measured value outside of the reference interval¹¹
- For these reasons, individual patient trending is more sensitive and better at detecting pathologic changes than reliance on published reference values for chemistry and hematology²⁰

Senior patients

- The common occurrence of physical exam and laboratory abnormalities in apparently healthy senior dogs and cats emphasizes the need for regular health screening, including regular laboratory testing^{12,13}
- Visit/exam frequency and testing recommendations should be based on patient's age, breed and lifestyle
- Senior and geriatric dogs and cats should be examined at least semiannually to allow for earlier intervention of chronic disease
- Regular testing at geriatric equine annual examinations assesses overall health and may display any early signs of potentially serious disease, such as liver and kidney dysfunction or onset of metabolic disease²¹





Responsible Patient Trending



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Keys to patient trending success


The best practice is to monitor a patient on the same analyzer using the same analytical methods

Whenever comparing or trending analyte results, it is important to trend using best practices and responsible trending to have a consistent comparison. This practice includes:


- Using the same analyzer every time, when possible
- Performing the test in the same way (sample type, number of hours pre- or posttreatment, fed or fasted state, etc)
- Keeping in mind that different assays and instruments have reference intervals that may differ among analyzers and/or laboratories
- Performing a quality check or verifying with a different test, methodology or laboratory if a value does not match the clinical picture

What is responsible trending?

Responsible Trending™, available only on the ZoetisDx online platform, shows chronological test analyte results as a sequence of graphs. **This visual format provides a clear story of each patient's trends in test results over time—with results from different analyzers displayed together but always relative to each analyte's reference interval on its respective analyzer.**

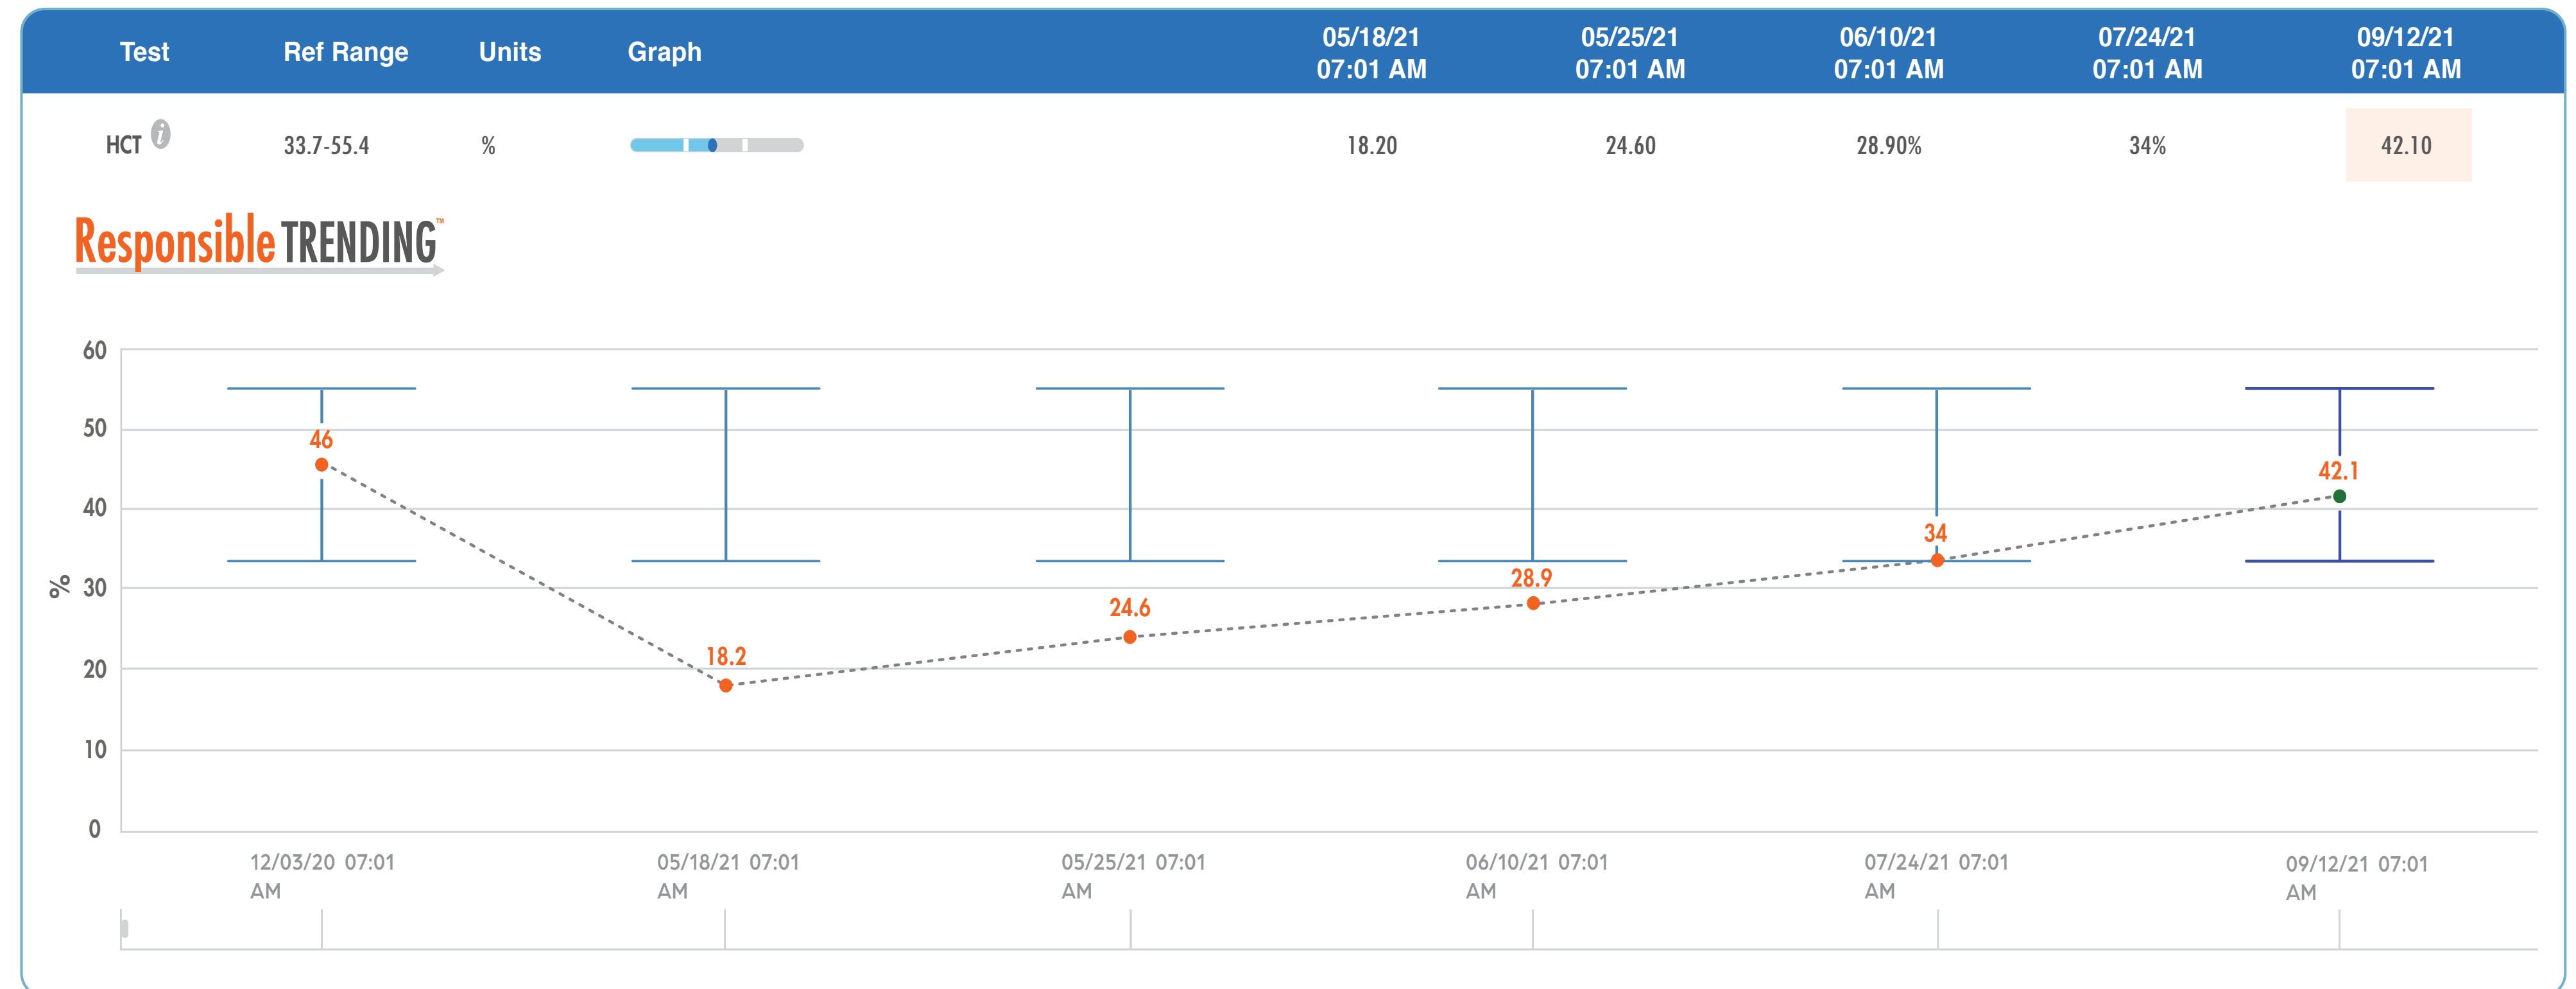

Note: It is imperative when comparing results between different analyzers or labs to interpret the raw value with respect to the reference interval provided and not the raw number due to inherent methodology differences.

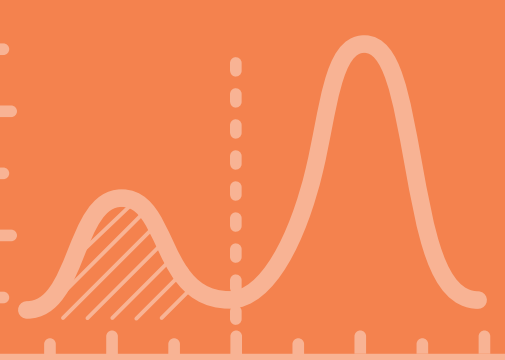

Histograms



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids


Reference Intervals (Ranges)

Introduction to histograms

Histograms are graphic representations of cell distribution and cell counts²²


Histograms are the graphs that display on your results screen or appear on the printed hematology report, depending on the practice management software used. They are easily understood and can help to:

Verify differential cell counts




The graphical display of data provides information not available in the automated CBC and allows verification of the CBC's numerical results

Perform quality control check



Show sample integrity and potential abnormalities, so users can quickly decide whether results are meaningful or whether they need to draw a new sample

Identify uncommon disease processes

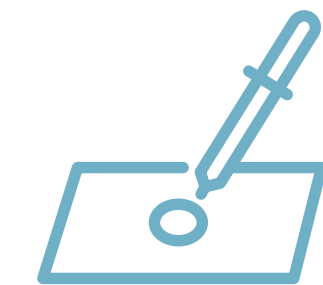

Identify uncommon disease processes that can affect cell morphology and distribution. These need to be confirmed visually with a blood smear

Histogram interpretation requires a thorough review of PLT, RBC and WBC curves for abnormalities

- Perform a blood smear for all patients who have any cell outside of the reference interval (range)
- Remember that a single hemogram is a snapshot in time and changes can occur rapidly
- Monitoring hemogram results frequently (every 12 to 24 hours) can be helpful in determining the course of an inflammatory response and response to treatment
- Always interpret results in conjunction with the clinical evaluation of the patient



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

[Interpreting histograms](#)

[Histogram examples](#)

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia


Alternative Fluids

Reference Intervals (Ranges)

Interpreting histograms

Histogram interpretation requires a thorough review of PLT, RBC and WBC curves for abnormalities.

Elements of a histogram²³

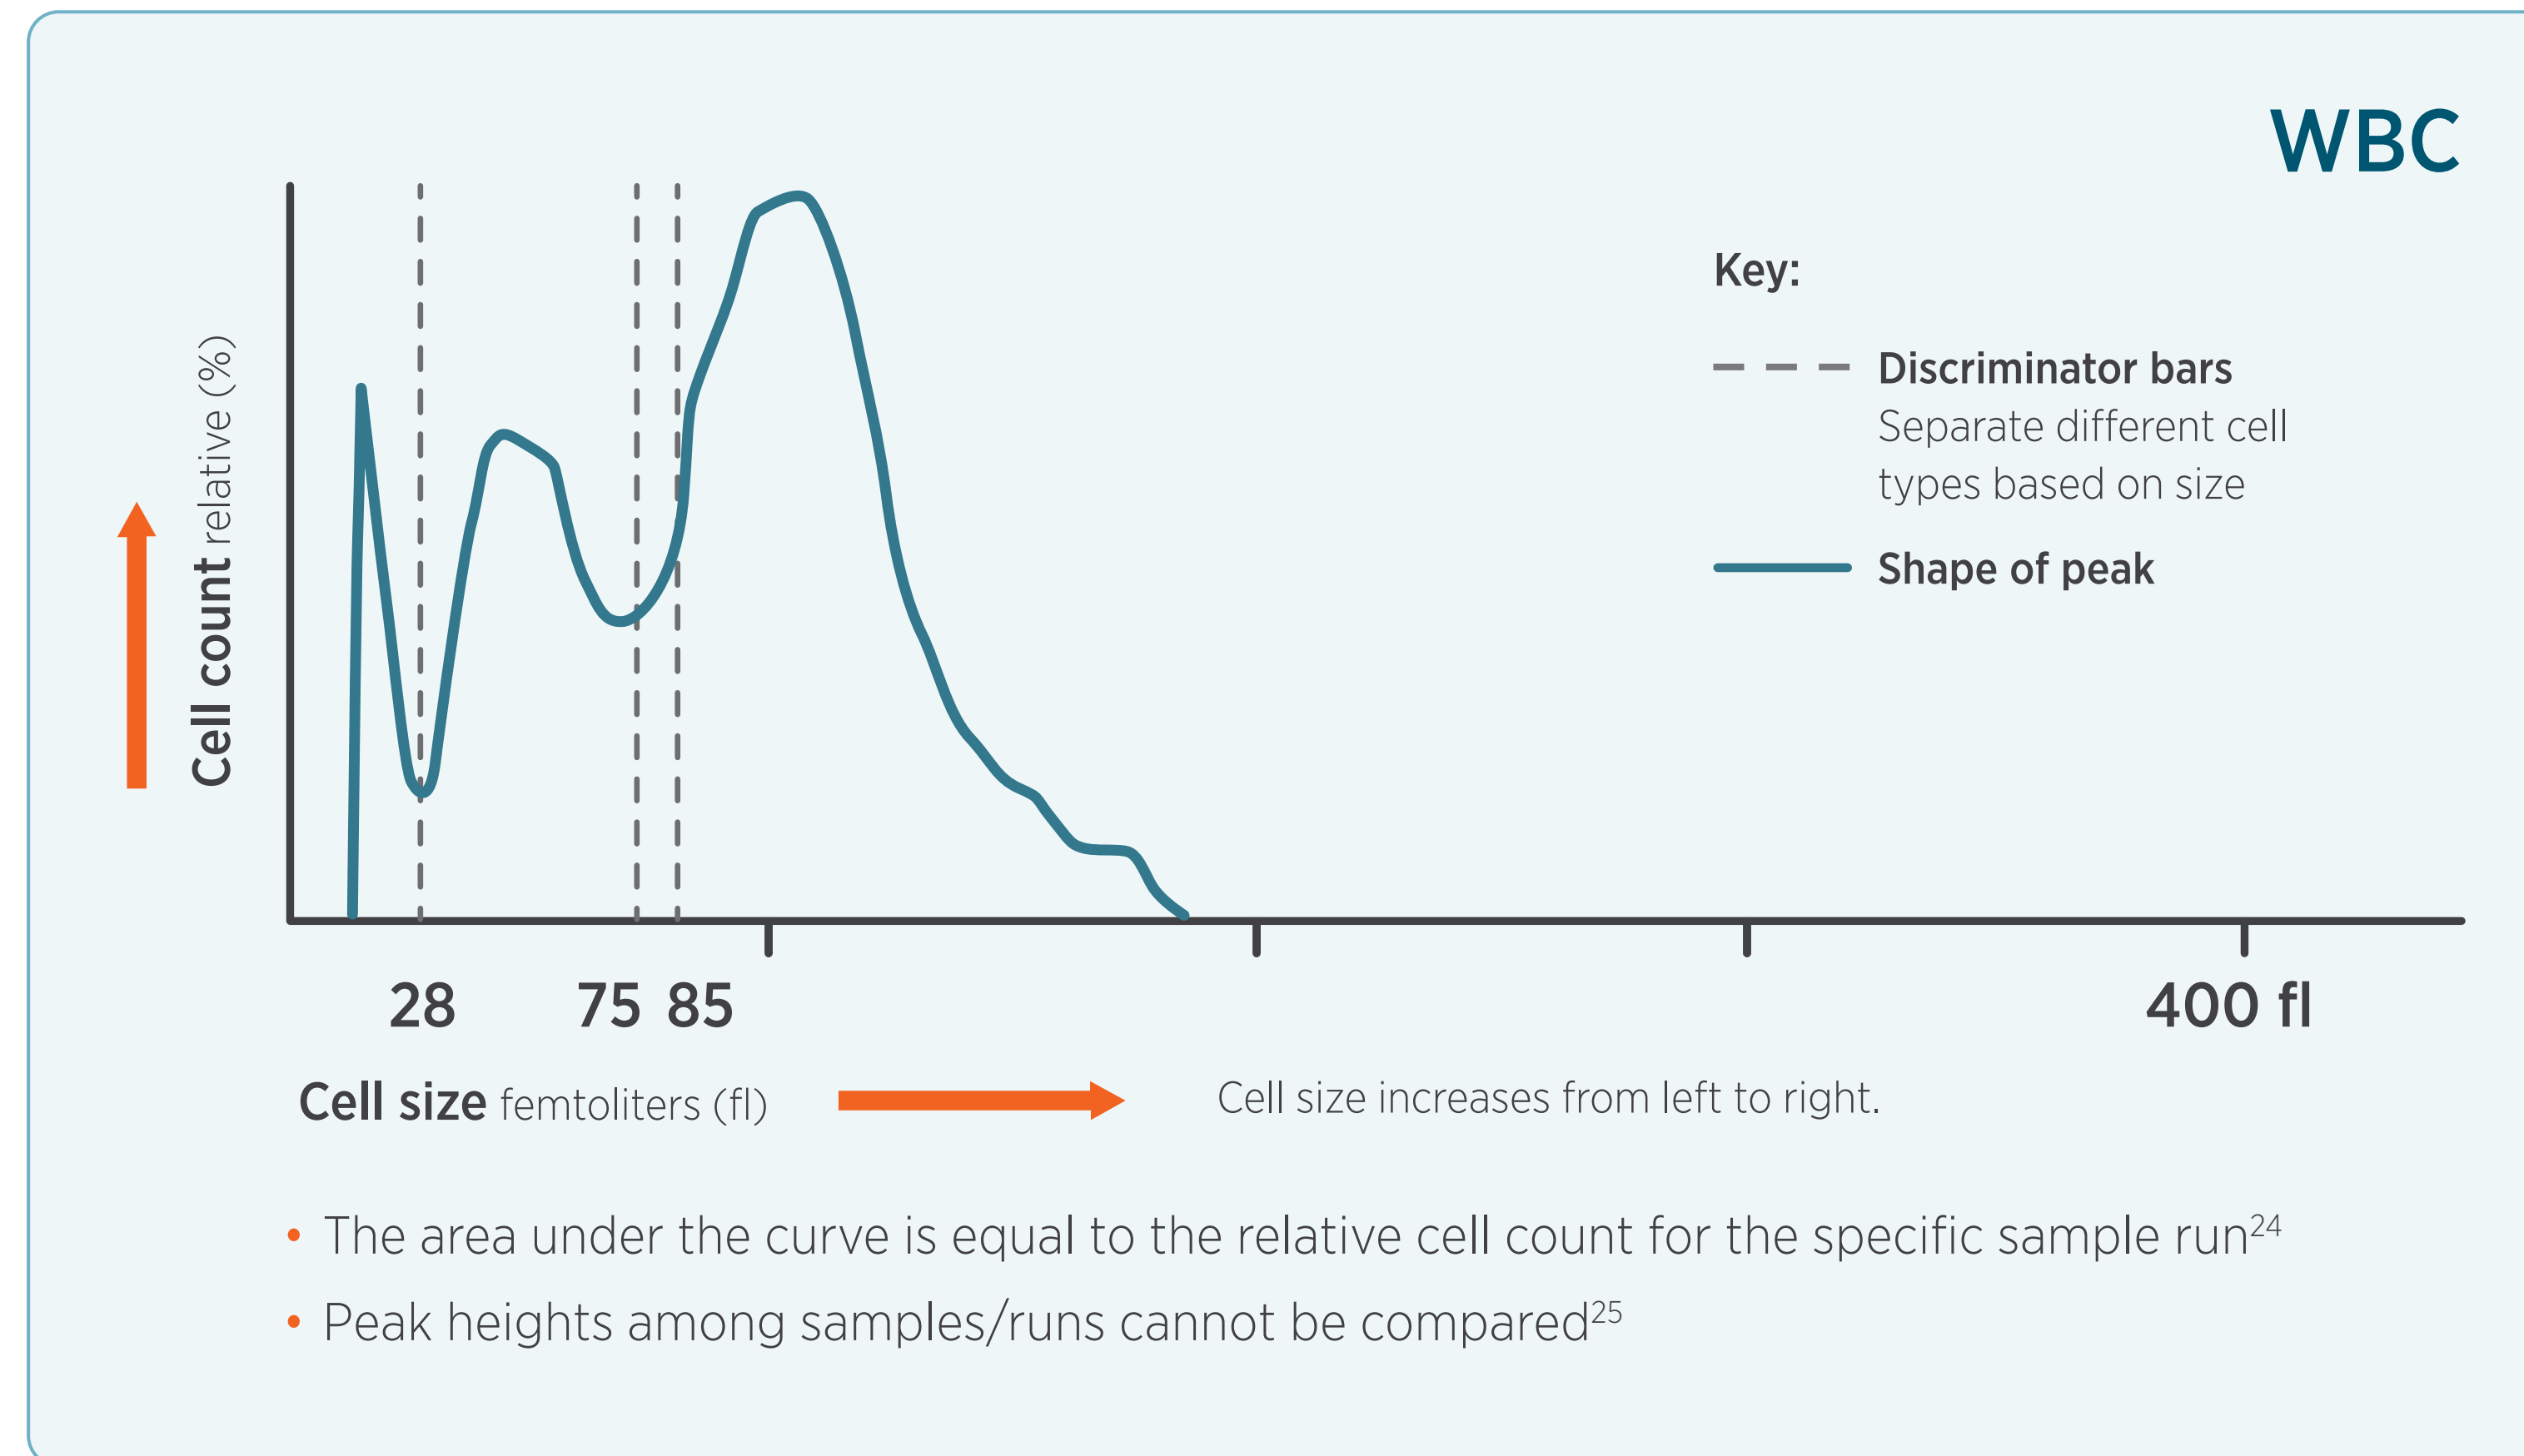

Histograms



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- [Interpreting histograms](#)
- Histogram examples

Interpretation Guide


- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Normal histograms

WBC Histogram

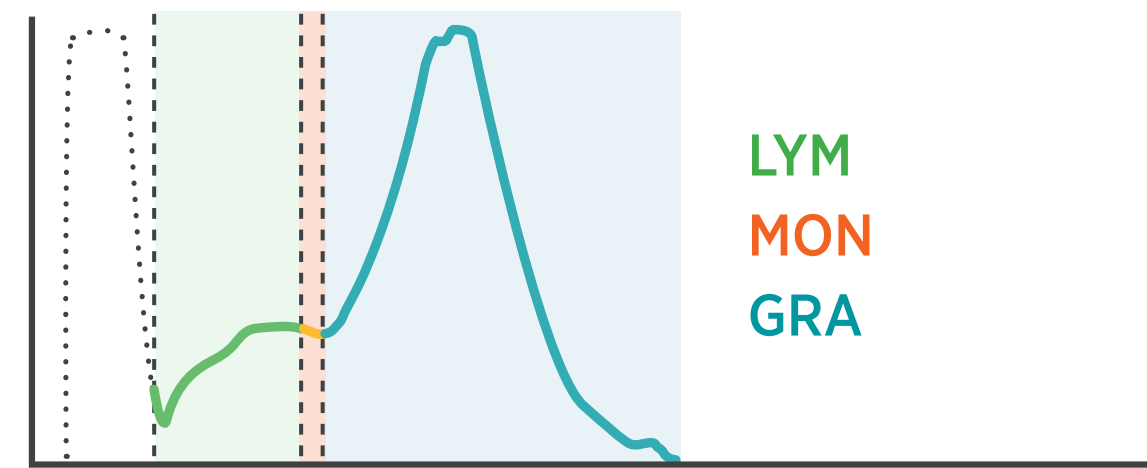


The peaks in the **WBC histogram**, separated by discriminators, correspond with LYM, MON and GRA. Debris (lysed RBC) from the WBC counting step may be seen to the left of the first discriminator.

LYM peak (left) is seen to the right of the first discriminator. In canines, the LYM peak starts on the low-to-mid portion along the y-axis, as shown, indicating lower populations of this cell type. In normal felines, peak starts on the mid portion of the y-axis due to higher relative number of LYM in cats

MON peak (center) is seen to the right of the second discriminator and is typically shorter due to a smaller population relative to other WBC

GRA peak (right) is seen to the right of the third discriminator and is predominantly composed of neutrophils. It is the tallest and widest peak, indicating it is the most numerous WBC population


EOS Histogram

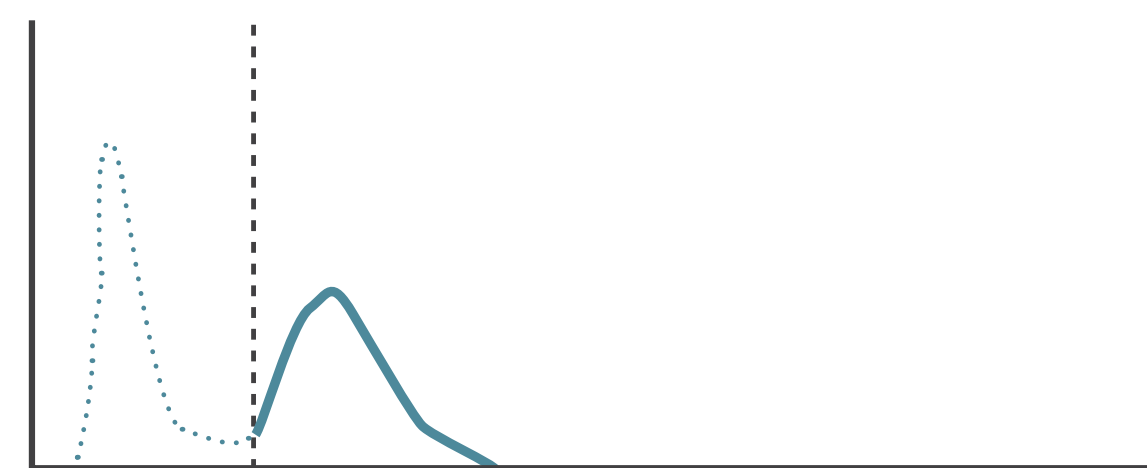

The **EOS histogram** varies and may be symmetrical or asymmetrical, jagged or smooth. Debris (lysed cells) from the EOS counting step may be seen to the left of the discriminator. It is not uncommon for the EOS discriminator to appear on the edge of the EOS peak.

- The eosinophils are counted separately from the other WBC types and are thus shown in a separate histogram
- Interpreting EOS by focusing on the numerical VETSCAN® HM5 data is recommended


RBC Histogram

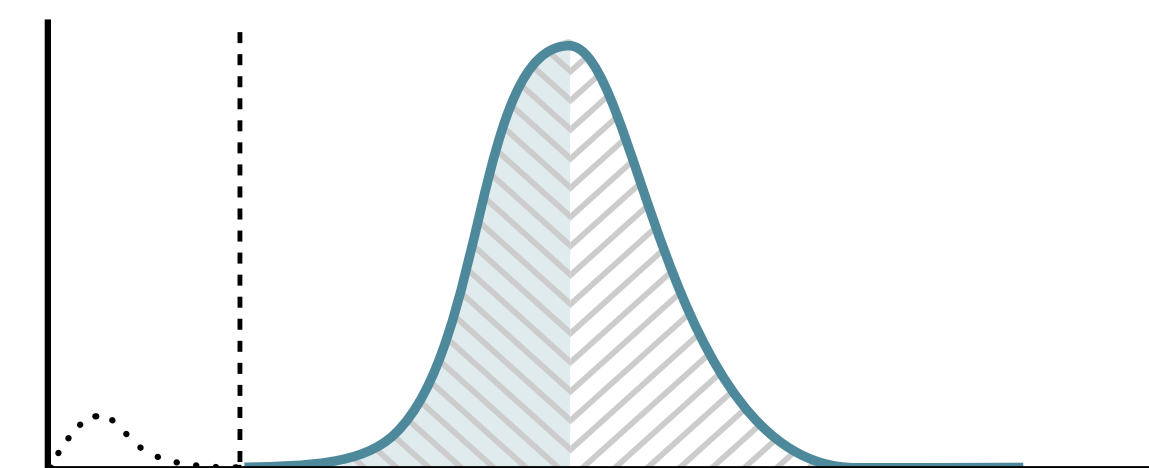

The **RBC histogram** in normal dogs and cats should present as an almost symmetrical, bell-shaped curve. The PLT peak can be seen to the left of the discriminator.

- The width of the curve relates to the RDWc
- An increased RDWc would show on the RBC histogram as a wider peak and mean that some of the RBC are either larger and/or smaller than normal
- RDWc measures anisocytosis, or RBC size variation

PLT Histogram

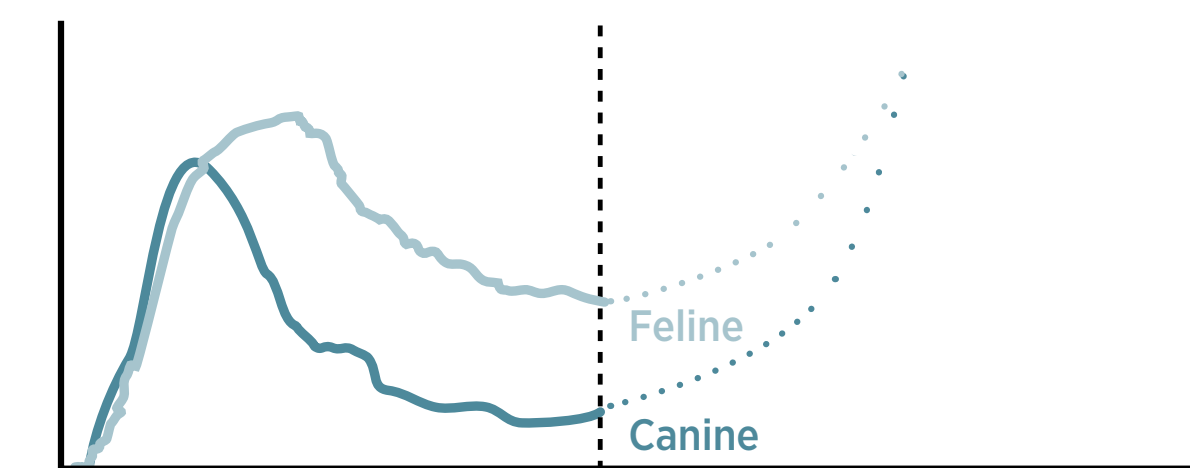

The **PLT histogram** begins with a sharp increase to a peak and tapers downward as cell size increases. This indicates that most PLT are small, with fewer large PLT. The RBC peak can be seen starting to the right of the discriminator.

- In felines and equines, the histogram tapers downward more slowly, indicating more large cells, commonly associated with mild PLT clumping
- The reported PLT number is the minimum number of free PLT counted by the analyzer
- The PLT histogram should be evaluated whenever the PLT count is low and/or lymphocytes are elevated. A blood smear to confirm a low PLT count is also recommended

RDWc=red cell distribution width (percent).

Histograms



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms

Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Histogram examples



PLT clumping and anemia²⁶
Feline

Always confirm these results with a blood smear



Histograms



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Histogram examples



Classic leukemia²⁶
Canine

Always confirm these results with a blood smear and potential pathology review



M warning flag may appear (refer to manual)

Histograms



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

Interpreting histograms

[Histogram examples](#)

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia


Alternative Fluids

Reference Intervals (Ranges)


Histogram examples



Microcytic anemia²⁵
Canine

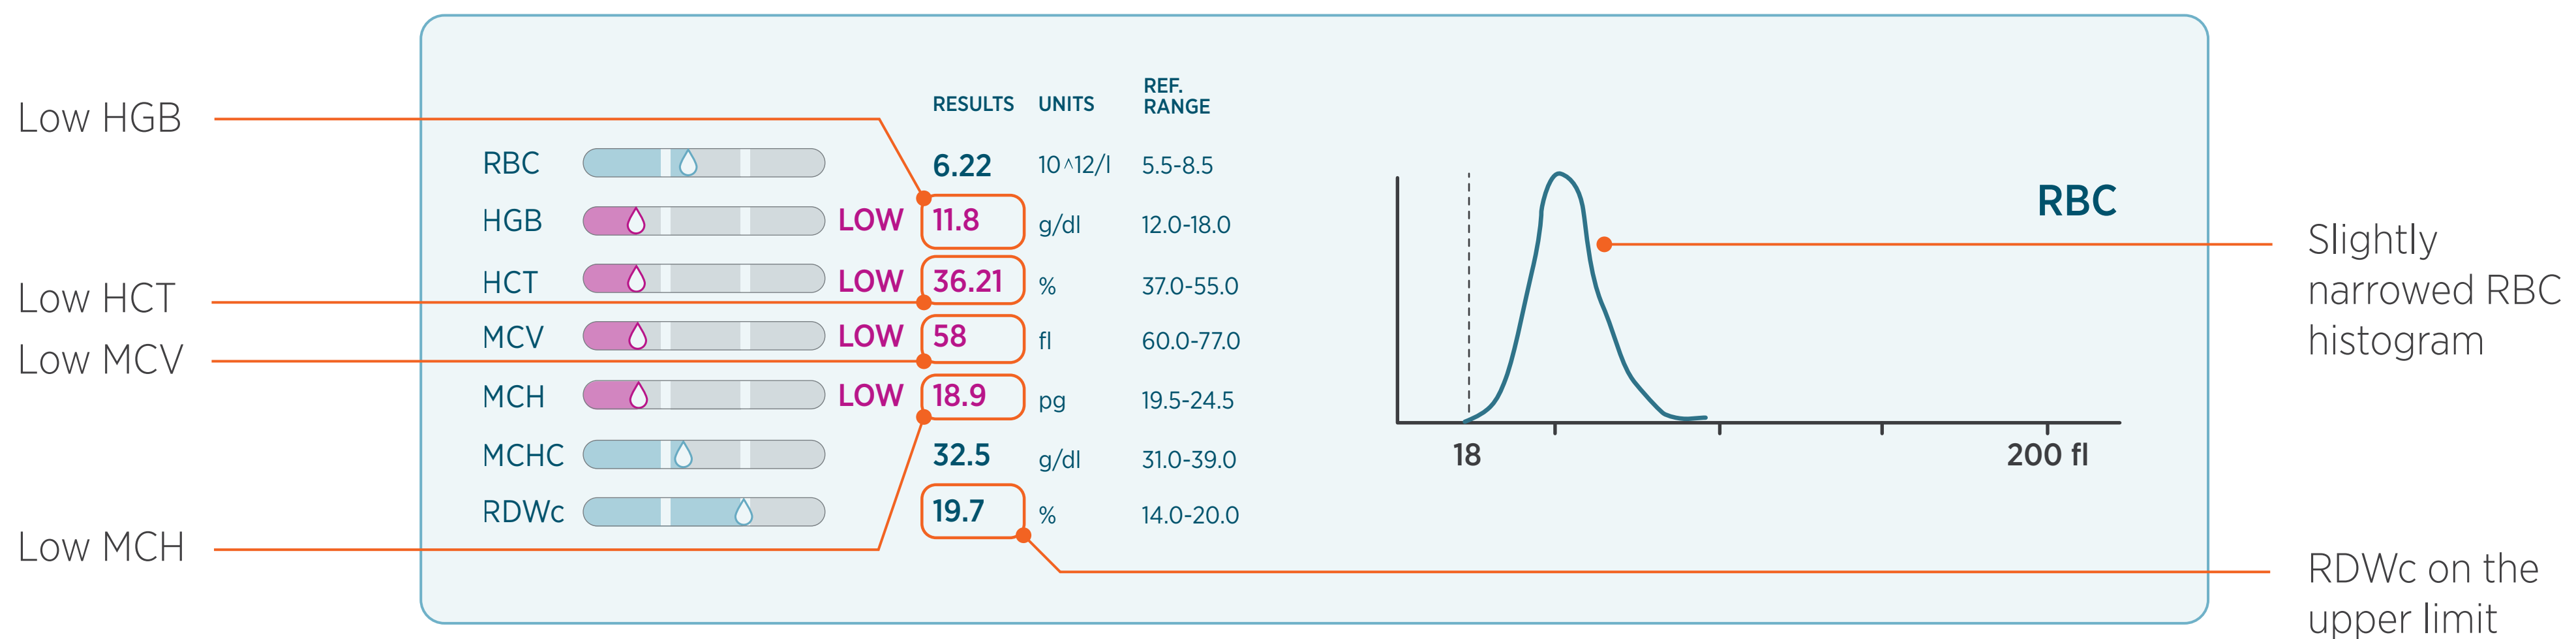

Stress leukogram²⁶
Canine

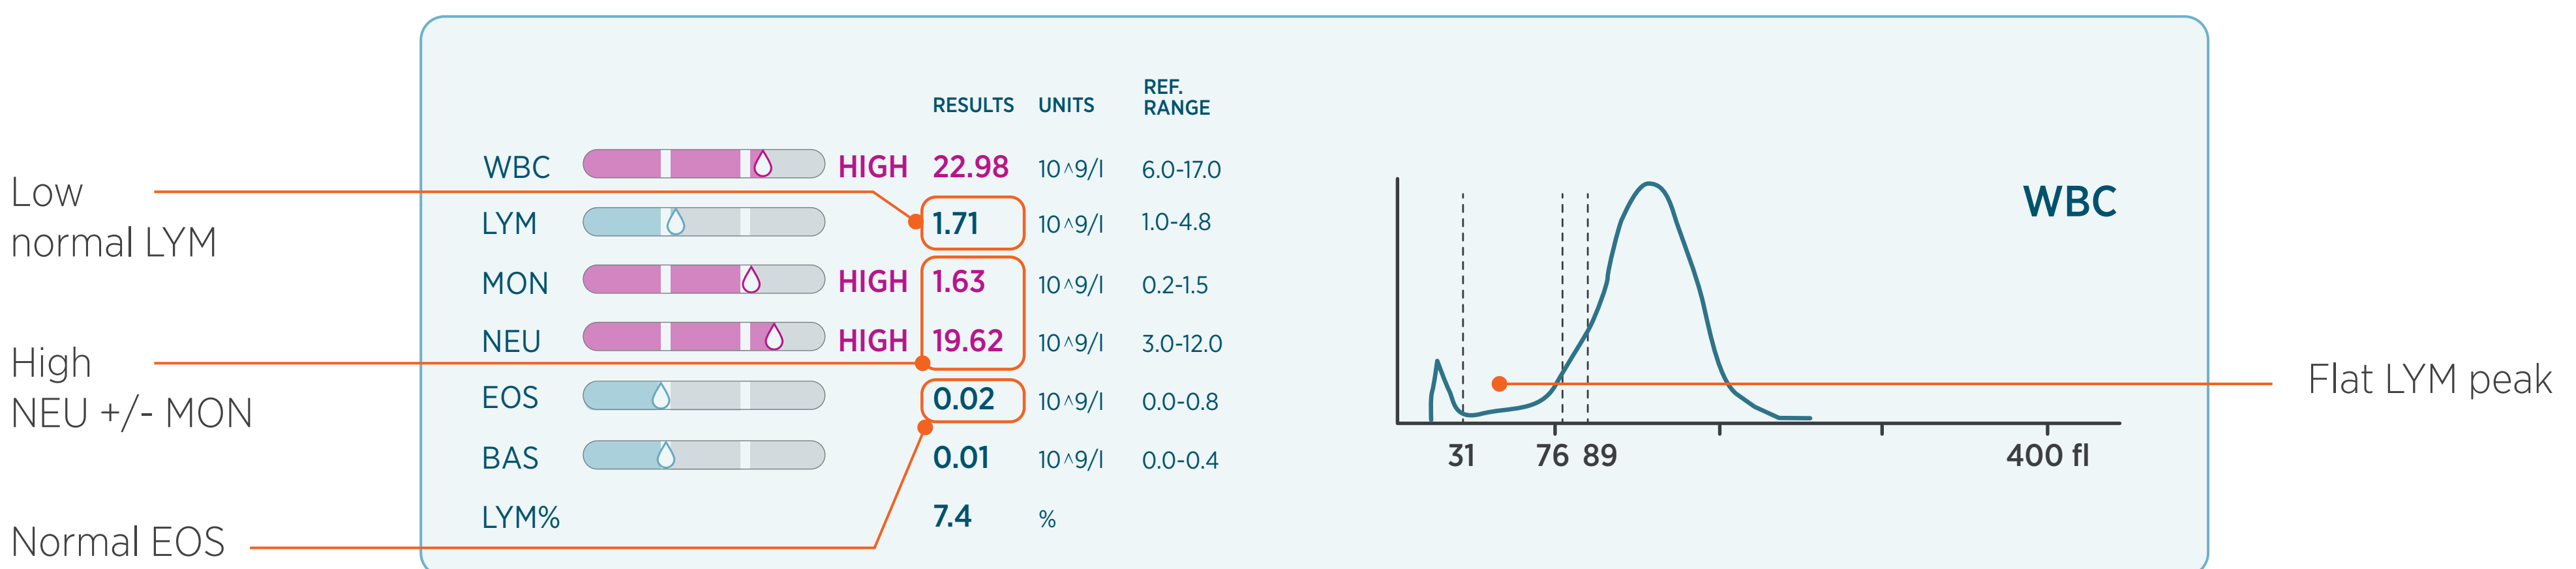



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

Macrothrombocytopenia

- Leukogram patterns
- Understanding anemia

Alternative Fluids


Reference Intervals (Ranges)

Inherited macrothrombocytopenia^{14,27}

Inherited macrothrombocytopenia is due to a mutation in the gene encoding beta1-tubulin. This mutation has been identified in approximately 90% of Cavalier King Charles spaniels (CKCSs), as well as other breeds, including bichons frises, boxers, cairn terriers, Chihuahuas, cocker spaniels, English toy spaniels, Havanese, Jack Russell terriers, labradoodles, Labrador retrievers, Maltese, mixed breeds, Norfolk terriers, poodles and shih tzu.

Inherited macrothrombocytopenia on the VETSCAN® HM5^{28,29}

Macrothrombocytes will not break into fragments when exposed to lyse solution and may cause inaccurate counts and/or instrument errors, particularly in analyzers that use impedance technology as the primary measurement method. When such samples are analyzed on the VETSCAN HM5, an “L” flag will often be displayed. While an “L” flag could suggest a potential lyse-resistant RBC anomaly or a problem with lyse delivery, in this case, the analyzer is reporting macroplatelets as nonlysed lymphocytes.

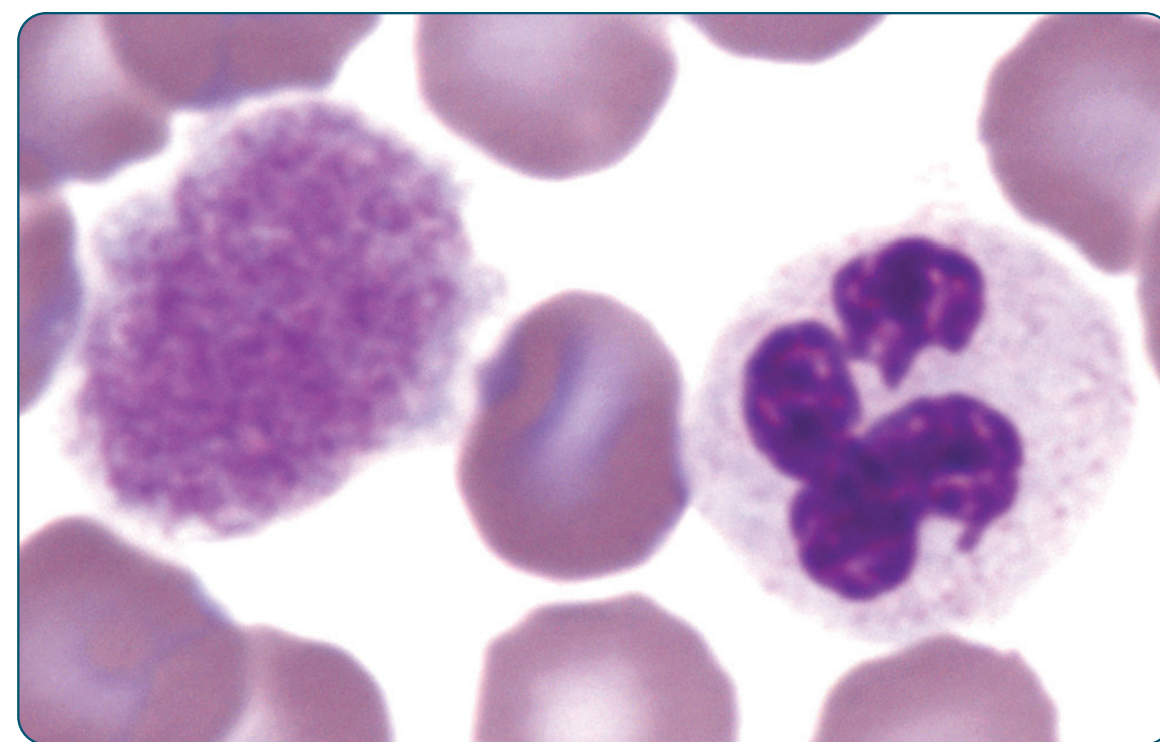


From chapter 7, Evaluation of hemostasis: coagulation and platelet disorders. Figure 7-26. In: Harvey JW, ed. *Veterinary Hematology: A Diagnostic Guide and Color Atlas*. 1st ed. Elsevier Inc.; 2012:211.

MPV=mean platelet volume.

A CBC from the VETSCAN HM5 for a patient with inherited macrothrombocytopenia will typically show an elevated LYM and a warning “L” flag

There will not be a significant PLT peak, and the PLT count will be reported as very low

The MPV may also be reported as normal

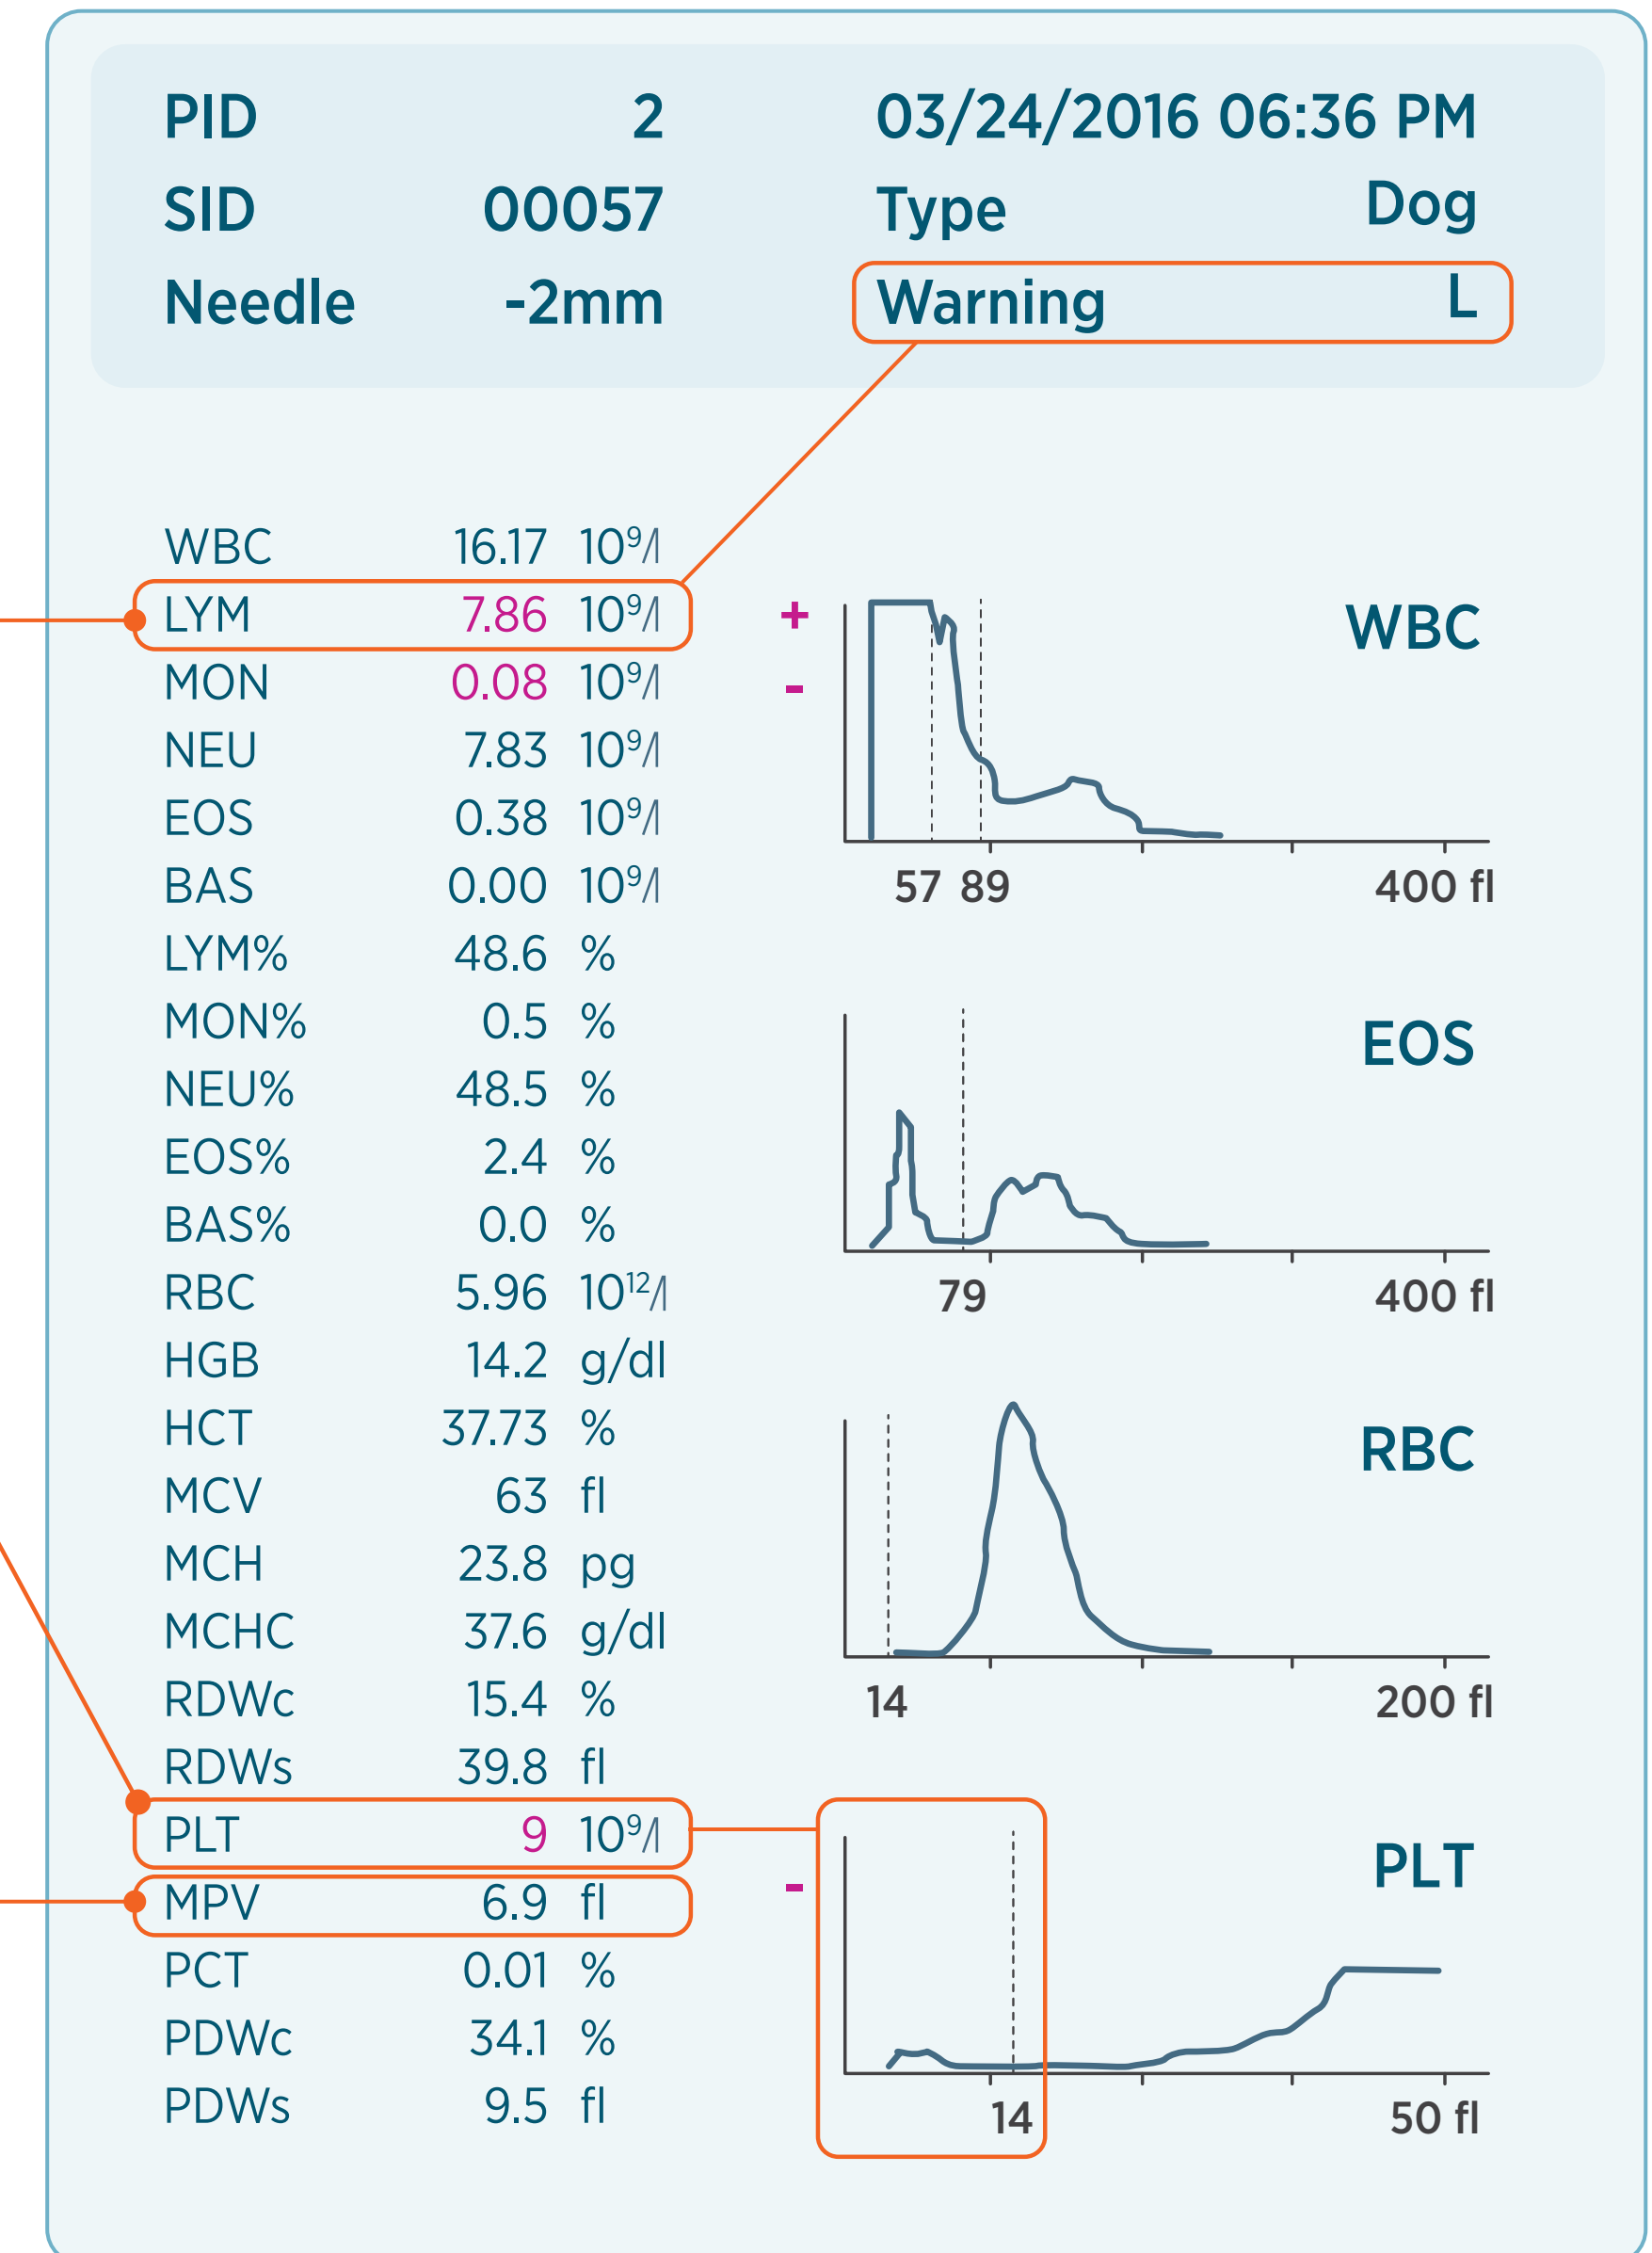

Note: Not every CKCS has macrothrombocytopenia. Those individuals with normal-size PLT will not show the features mentioned above.



Interpretation Guide



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)


Understanding classic leukogram patterns

Changes in total and differential leukocyte counts are usually grouped into patterns that facilitate interpretation. These patterns are:

		NEU	Left Shift	Toxic Δ^*	LYM	MON	Inflammation
Stress leukogram	<ul style="list-style-type: none"> A result of cortisol released by the adrenal gland Occurs due to a wide range of processes <ul style="list-style-type: none"> — Systemic illness; metabolic disturbance; pain Mimicked by corticosteroid therapy 	↑	No	No	↓	↑ canine > feline	+/-
Physiological leukocytosis	<ul style="list-style-type: none"> A result of epinephrine or norepinephrine release Also called a flight-or-fight response Most often seen in cats (of any age) and possibly in the young of other species Usually transient and generally resolves about 30 minutes after the patient relaxes 	↑	No	No	↑ (mostly feline)	Normal	Unusual
Inflammatory leukogram	<ul style="list-style-type: none"> Represents the balance between tissue demand and bone marrow supply May vary depending on source and severity of inflammation and timing of sample collection NEU numbers may vary from severely depressed to markedly increased A left shift indicates the presence of immature NEU <ul style="list-style-type: none"> — Usually, but not always, indicates an inflammatory leukogram Inflammation is possible in patients without an inflammatory leukogram 	Mild/Chronic Inflammation					
		↑	+/-	No	Normal or ↓	↑ (chronic)	Hopefully
		Acute Inflammation					
		↑	↑	Frequent	↓	Normal or ↑	Yes
Overwhelming Inflammation							
↓	↑ to ↑↑	Present	↓	No	Yes		
Leukemoid reaction	<ul style="list-style-type: none"> Characterized by a marked neutrophilic leukocytosis (>50,000 cells/μL) with a concurrent, orderly left shift Toxic changes may or may not be present Resembles granulocytic leukemia but is caused by another process Also referred to as extreme neutrophilic (granulocytic) leukocytosis 	↑↑↑	+/-	Occasional	Normal or ↓	Normal or ↑	?

* Δ =change.

[See more detailed information on inflammatory patterns](#) ↗

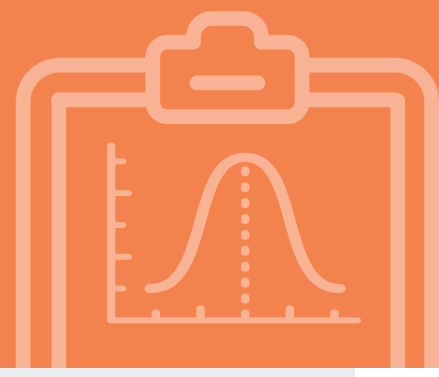

How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Understanding anemia


Anemia is one of the most common hematologic abnormalities encountered in veterinary clinical practice. It is the manifestation of an underlying disorder, like a fever, and not a diagnosis. It can be a primary sign of disease (eg, hemorrhage or immune-mediated hemolytic anemia) or a marker of underlying disease (eg, cancer or chronic kidney disease). Therefore, even mild, asymptomatic anemia should be investigated thoroughly to diagnose and treat the primary problem.

Anemia is defined by a PCV, HCT, HGB or RBC count below the reference intervals for that species. Anemia can be mild, moderate or severe and could be caused by an acute disease process or have been ongoing for a long time due to a chronic condition.


When evaluating an anemic patient, hematology testing MUST include BOTH quantitative automated cell count + qualitative blood smear evaluation

Once we receive abnormal RBC, HCT, HGB or PCV results, how do we proceed?

- Evaluate the hematology results in the context of the entire patient, including the patient's signalment and clinical status as well as the minimum database and other diagnostic tests
- Consider the potential for laboratory or sampling error
- If an automated count is performed and anemia detected:
 - Confirm with a PCV, since this is the direct measurement of the proportion of blood comprised of RBC
 - Perform a blood smear to examine the RBC morphology and confirm automated cell counts to aid in determining a diagnosis and prognosis
- Remember, a comprehensive CBC includes an automated cell count along with a blood smear evaluation

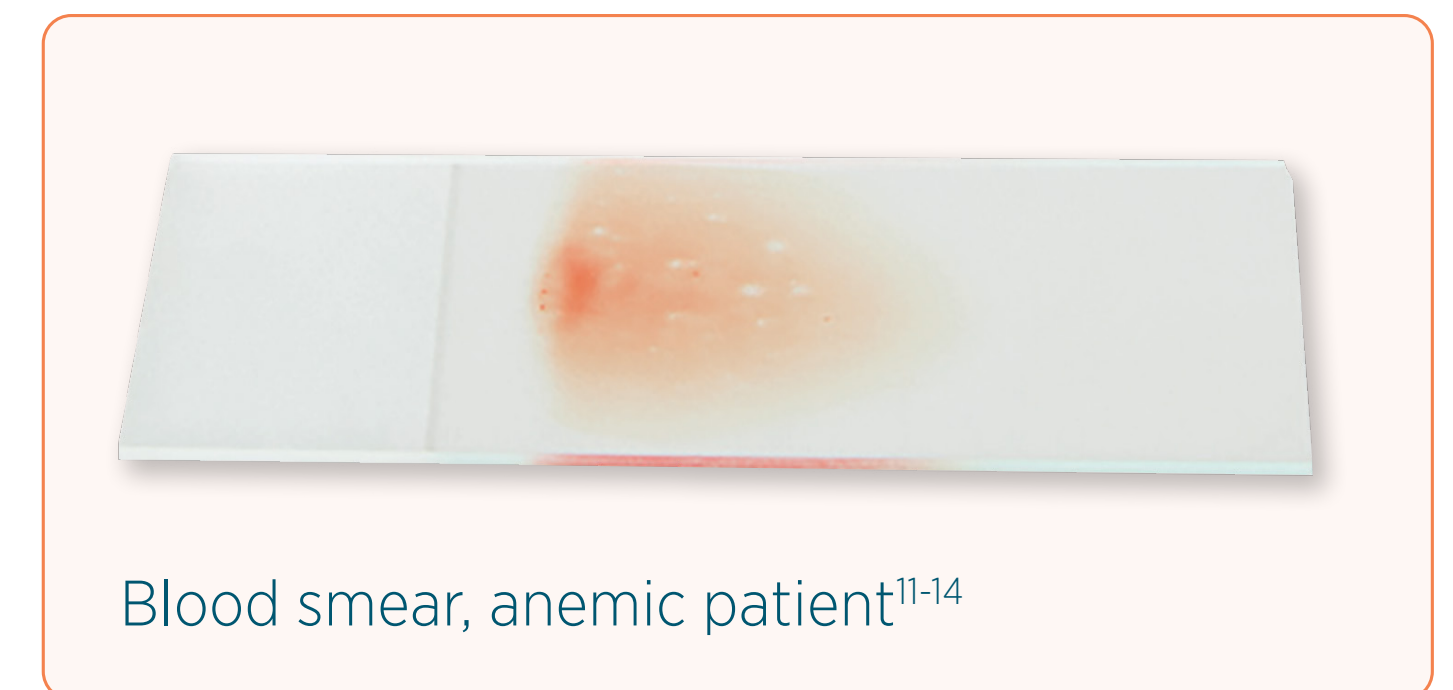

Note: Anemia can be masked by concomitant dehydration. Decreased measured erythrocyte parameters may also be observed when the total-body erythrocyte mass is normal but there is an expansion of the vascular space faster than the expansion of the total-body erythrocyte mass (relative anemia).³⁰⁻³²

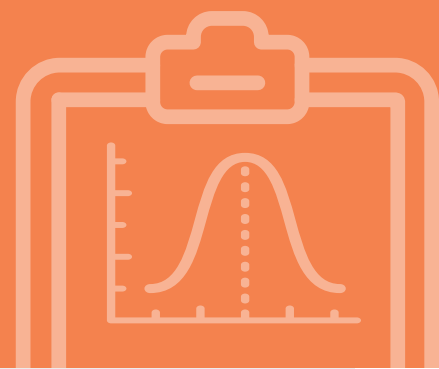

How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Further diagnostic testing to determine the underlying cause of anemia³³

Blood smear examination provides information about blood cell pathology and the potential for blood parasites not available with automated analyzers. In addition, evaluation of RBC morphology can help pinpoint a diagnosis, determine the recommended treatment and monitor the response to treatment for anemia.

Common RBC morphologies

IMHA	Regenerative anemia	RBC damage due to microangiopathy*	Oxidative damage	Iron deficiency
Spherocytes	Anisocytosis	Schistocytes	Eccentrocytes	Schistocytes
Agglutination	Howell-Jolly bodies	Acanthocytes	Heinz bodies	Microcytes
Ghost cells	Polychromasia	Keratocytes	Spherocytes	Leptocytes

*Associated with neoplasia, disseminated intravascular coagulation, glomerulonephritis or vasculitis.

Consider the whole patient

Because anemia is a manifestation of an underlying disorder and not a diagnosis, further diagnostic testing is usually necessary to determine the underlying cause. Additional diagnostic tests listed below should be utilized based on the differential diagnosis suggested by the classification of anemia (see **Anemia algorithm** on page 26).

Additional diagnostic tests

- Clinical chemistry profile/urinalysis +/- endocrine testing
- Virology, serology if infection is likely (eg, fever, lymphadenopathy, etc)
- Bone marrow examination may reveal many diagnoses (eg, myelofibrosis, aplastic anemia, bone marrow necrosis/inflammation, dyserythropoiesis, leukemia, metastatic neoplasia, myelodysplastic syndromes, etc)

IMHA=immune mediated hemolytic anemia.



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia


Alternative Fluids

Reference Intervals (Ranges)

Two ways to classify anemia: bone marrow responsiveness


- Classification of anemia in accordance with bone marrow responsiveness is based on the presence or absence of an increased number of immature erythrocytes in circulation (known as reticulocytosis, polychromasia) or erythroid hyperplasia in the bone marrow. Evaluation must be interpreted relative to the duration and severity of the anemia³²
- In most species, a RETIC count is considered the easiest, most reliable measure of marrow responsiveness. A notable exception is the horse, which releases few to no immature RBC into circulation; therefore, a bone marrow sample must be used to determine the erythroid response
 - Note:** an automated RETIC count should always be verified with a blood smear to examine RBC morphology and to confirm the automated RETIC count

RETIC counts can be interpreted by either absolute or corrected counts to determine if regeneration exists

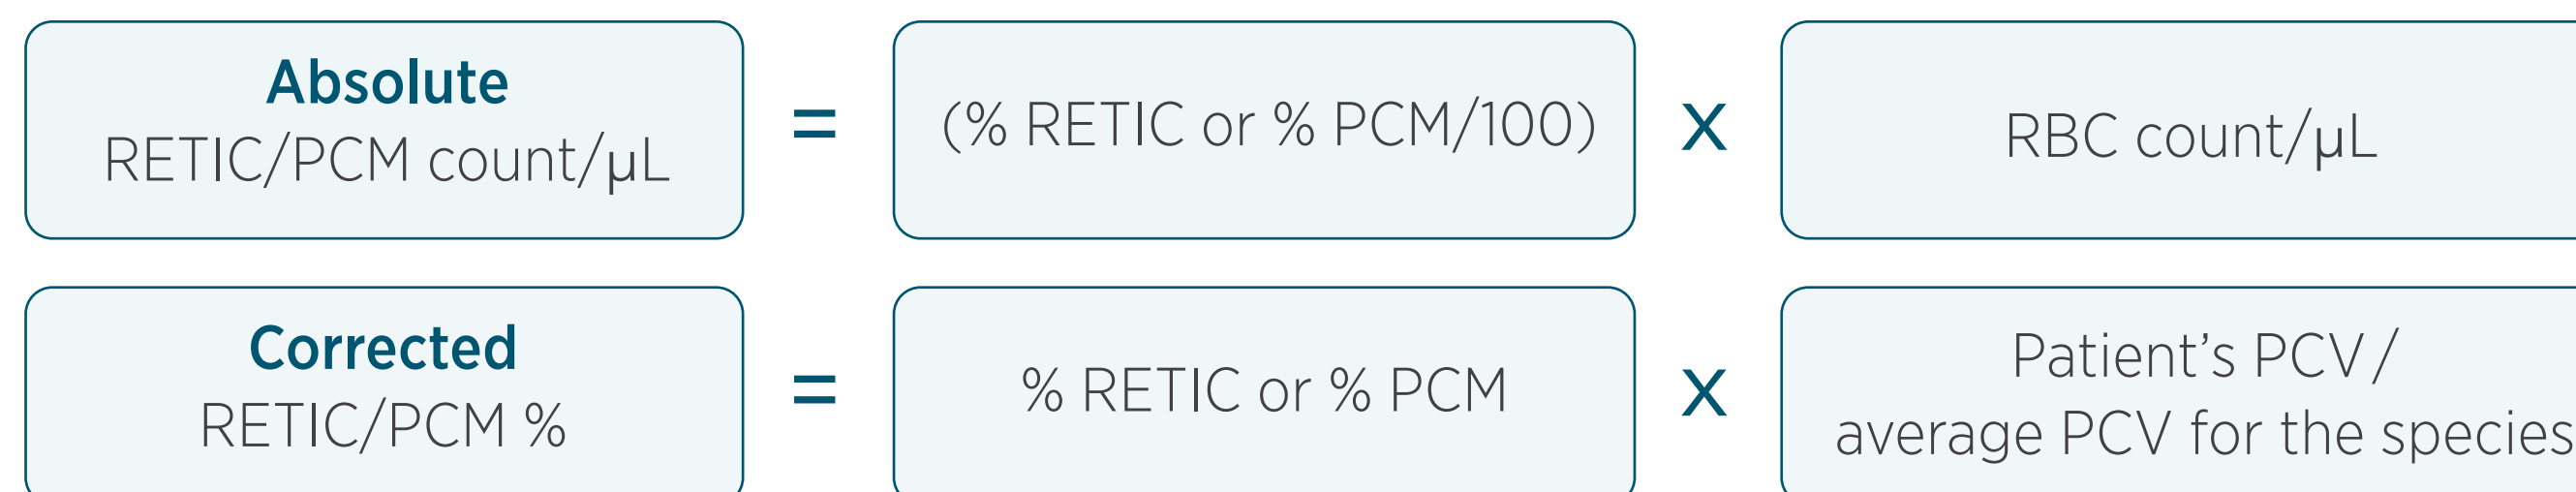

- Interpretation must be made relative to the duration and severity of the anemia. Simply relying on a reference interval may lead to misinterpretation of the erythroid response. See **Anemia algorithm** on page 26 for examples

VETSCAN IMAGYST™ can identify polychromatophils

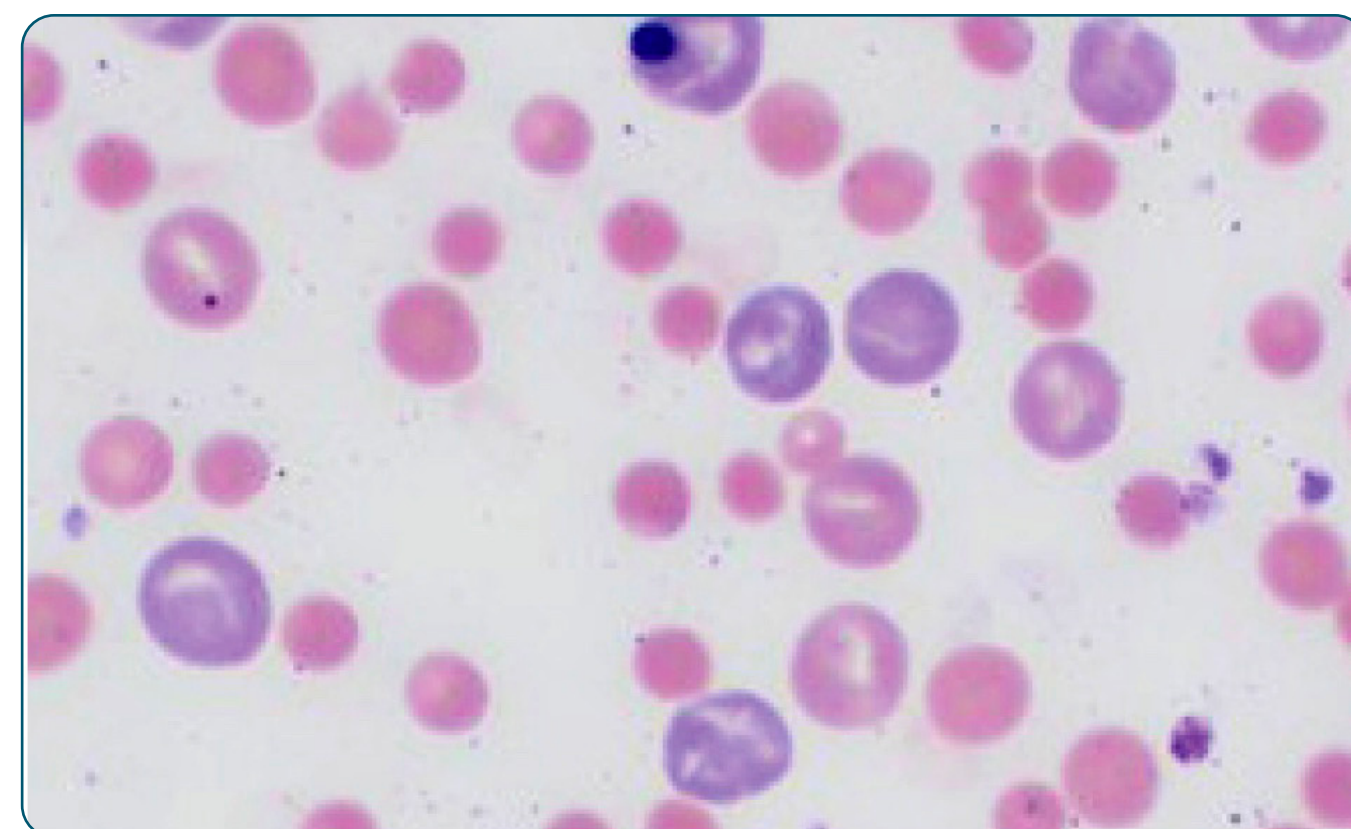

VETSCAN IMAGYST supports using a PCM count to classify the bone marrow response to an anemia. RETIC and PCM are both immature red blood cells and have the same function but are identified using different staining methodologies.

Image obtained from VETSCAN IMAGYST at 400x magnification, showing Wright's-stained blood smear of RBC. Immature RBC are shown in a purple-blue color.



Interpretation Guide



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns

Understanding anemia


Alternative Fluids

Reference Intervals (Ranges)

Two ways to classify anemia: bone marrow responsiveness


Anemia algorithm³⁴⁻³⁵

[See the full anemia algorithm](#) ↗

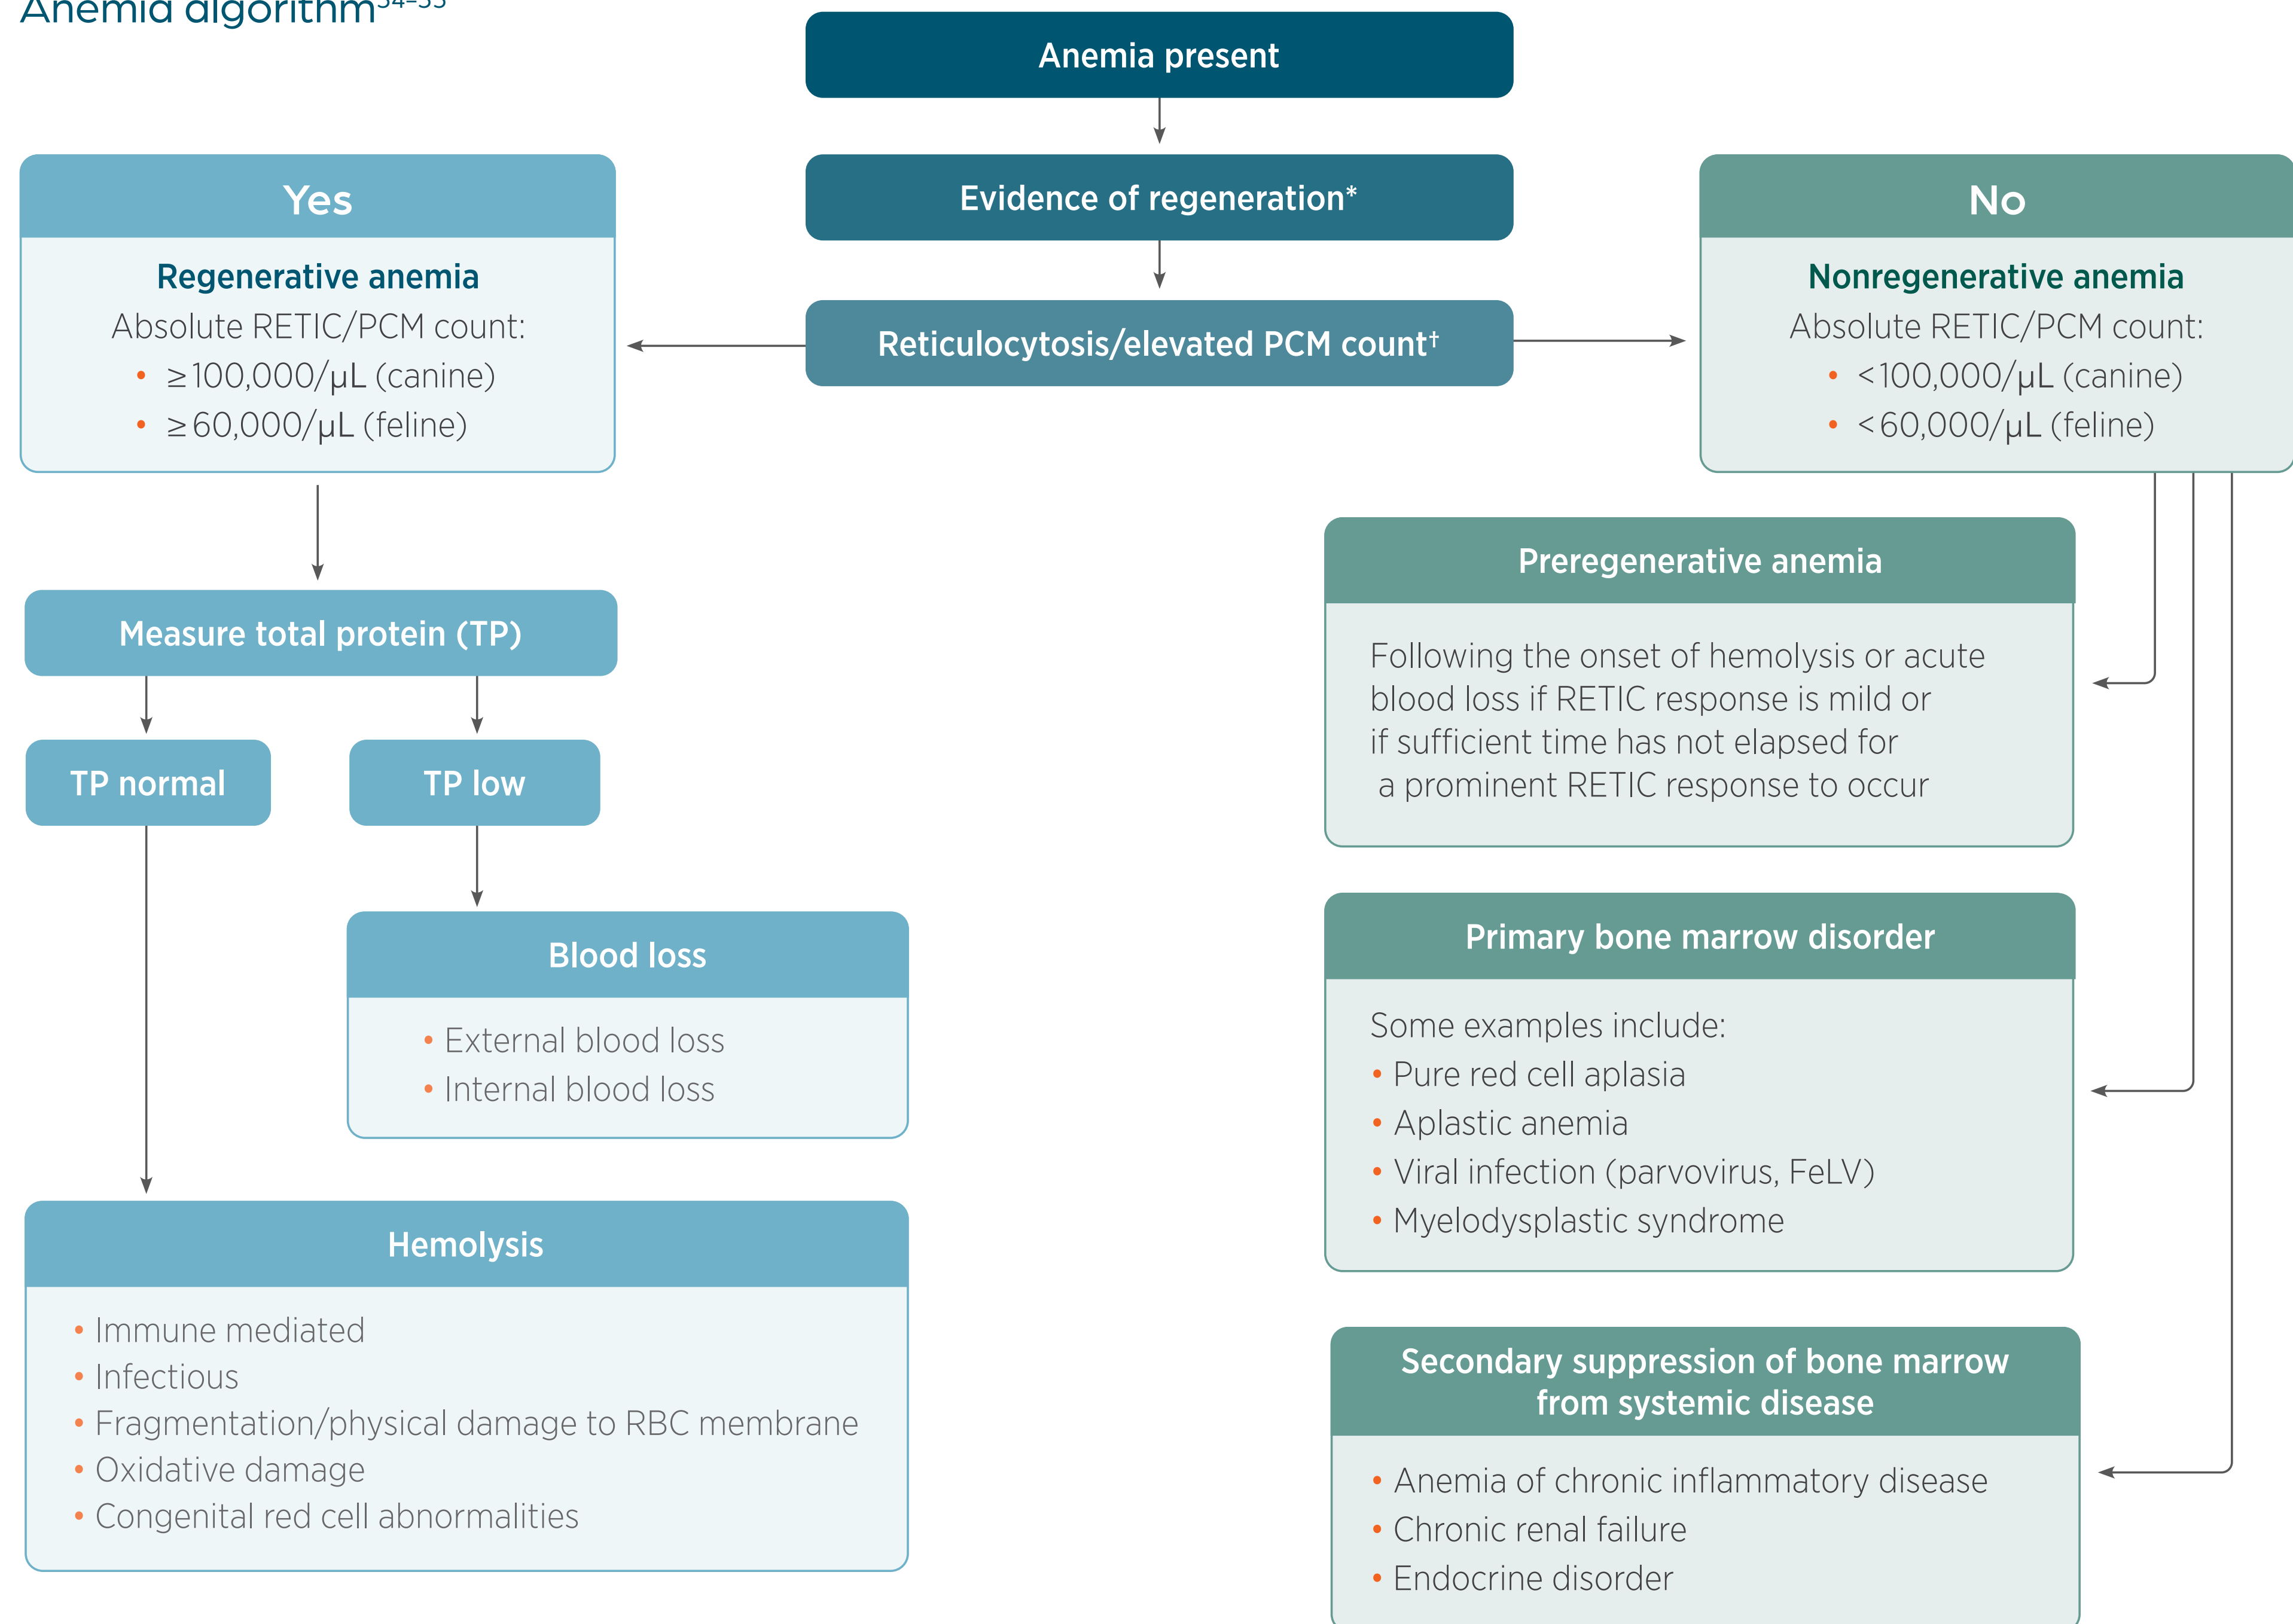

*Evaluation of the adequacy of the bone marrow regenerative response in the individual patient should also include consideration of severity and chronicity of the anemia, suspected cause of the anemia and potential for multiple causes contributing to the patient's anemia. Trending the anemia and RETIC/PCM count through sequential CBC may be helpful.

†RETIC/PCM counts supporting regeneration can be seen in nonanemic patients. This may reflect a normal physiological response or a response to an increased need. Serial evaluations of the CBC should be done to rule out an emerging anemia in these patients. RETIC or elevated PCM counts in the absence of anemia (RAA) may indicate recovery from anemia or may be associated with nonanemic chronic hypoxia (eg, cardiovascular disease, pulmonary disease). RAA has also been observed in patients with gastrointestinal, inflammatory and neoplastic disorders and in dogs with osteoarthritis or receiving osteoarthritis treatments (eg, anti-inflammatory drugs, nutraceuticals).

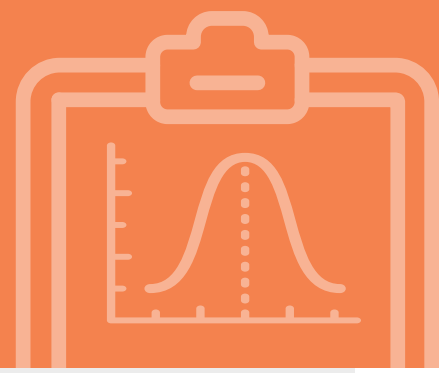

Interpretation Guide



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns

Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Two ways to classify anemia: red blood cell indexes


- In addition to RETIC or PCM counts, it is important to review the pertinent RBC parameters found on the automated CBC report: MCV and MCHC to describe trends in RBC size and HGB concentration to aid in classification of the anemia
- See **Anemia algorithm** on page 26 for additional information

Table: MCV classifications

MCV	Description	Common pathology
Decreased	Microcytic	<ul style="list-style-type: none"> Iron deficiency Hepatic portocaval vascular shunts Normal breed variation (eg, Shiba Inu, Akita)
Normal	Normocytic	<ul style="list-style-type: none"> Usually nonregenerative, poorly or early regenerative “Early regenerative” refers to blood loss or blood destruction anemia in which evidence of regeneration is not yet apparent because the bone marrow has not had time to respond to acute loss
Increased	Macrocytic	<ul style="list-style-type: none"> Regeneration: bone marrow is responding and is releasing PCM/RETIC that are larger than normal Congenital poodle macrocytosis Hereditary stomatocytosis Myelodysplasia FeLV


The 3 most important and relevant anemia diagnostic patterns using RBC indexes are³⁴:

Microcytic Hypochromic

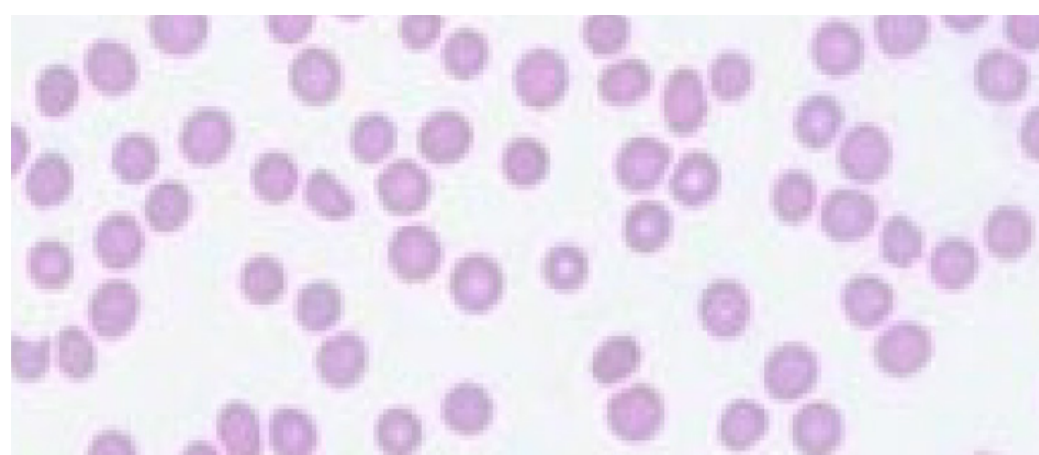

Usually due to iron deficiency anemias

Normocytic Normochromic

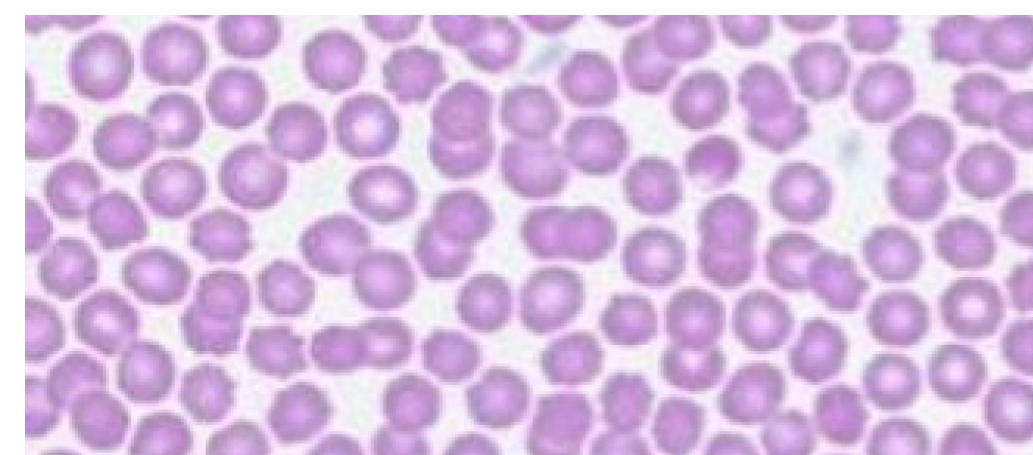


Nonregenerative anemias with residual normal erythrocytes

Macrocytic Hypochromic



Regenerative anemias with large, young erythrocytes that are not fully hemoglobinized


Images obtained from VETSCAN IMAGYST™.

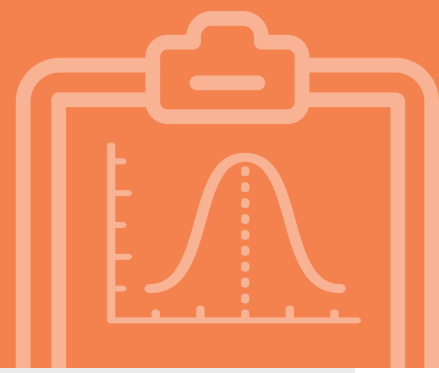

Interpretation Guide



Anemia classification by red blood cell indexes³⁵

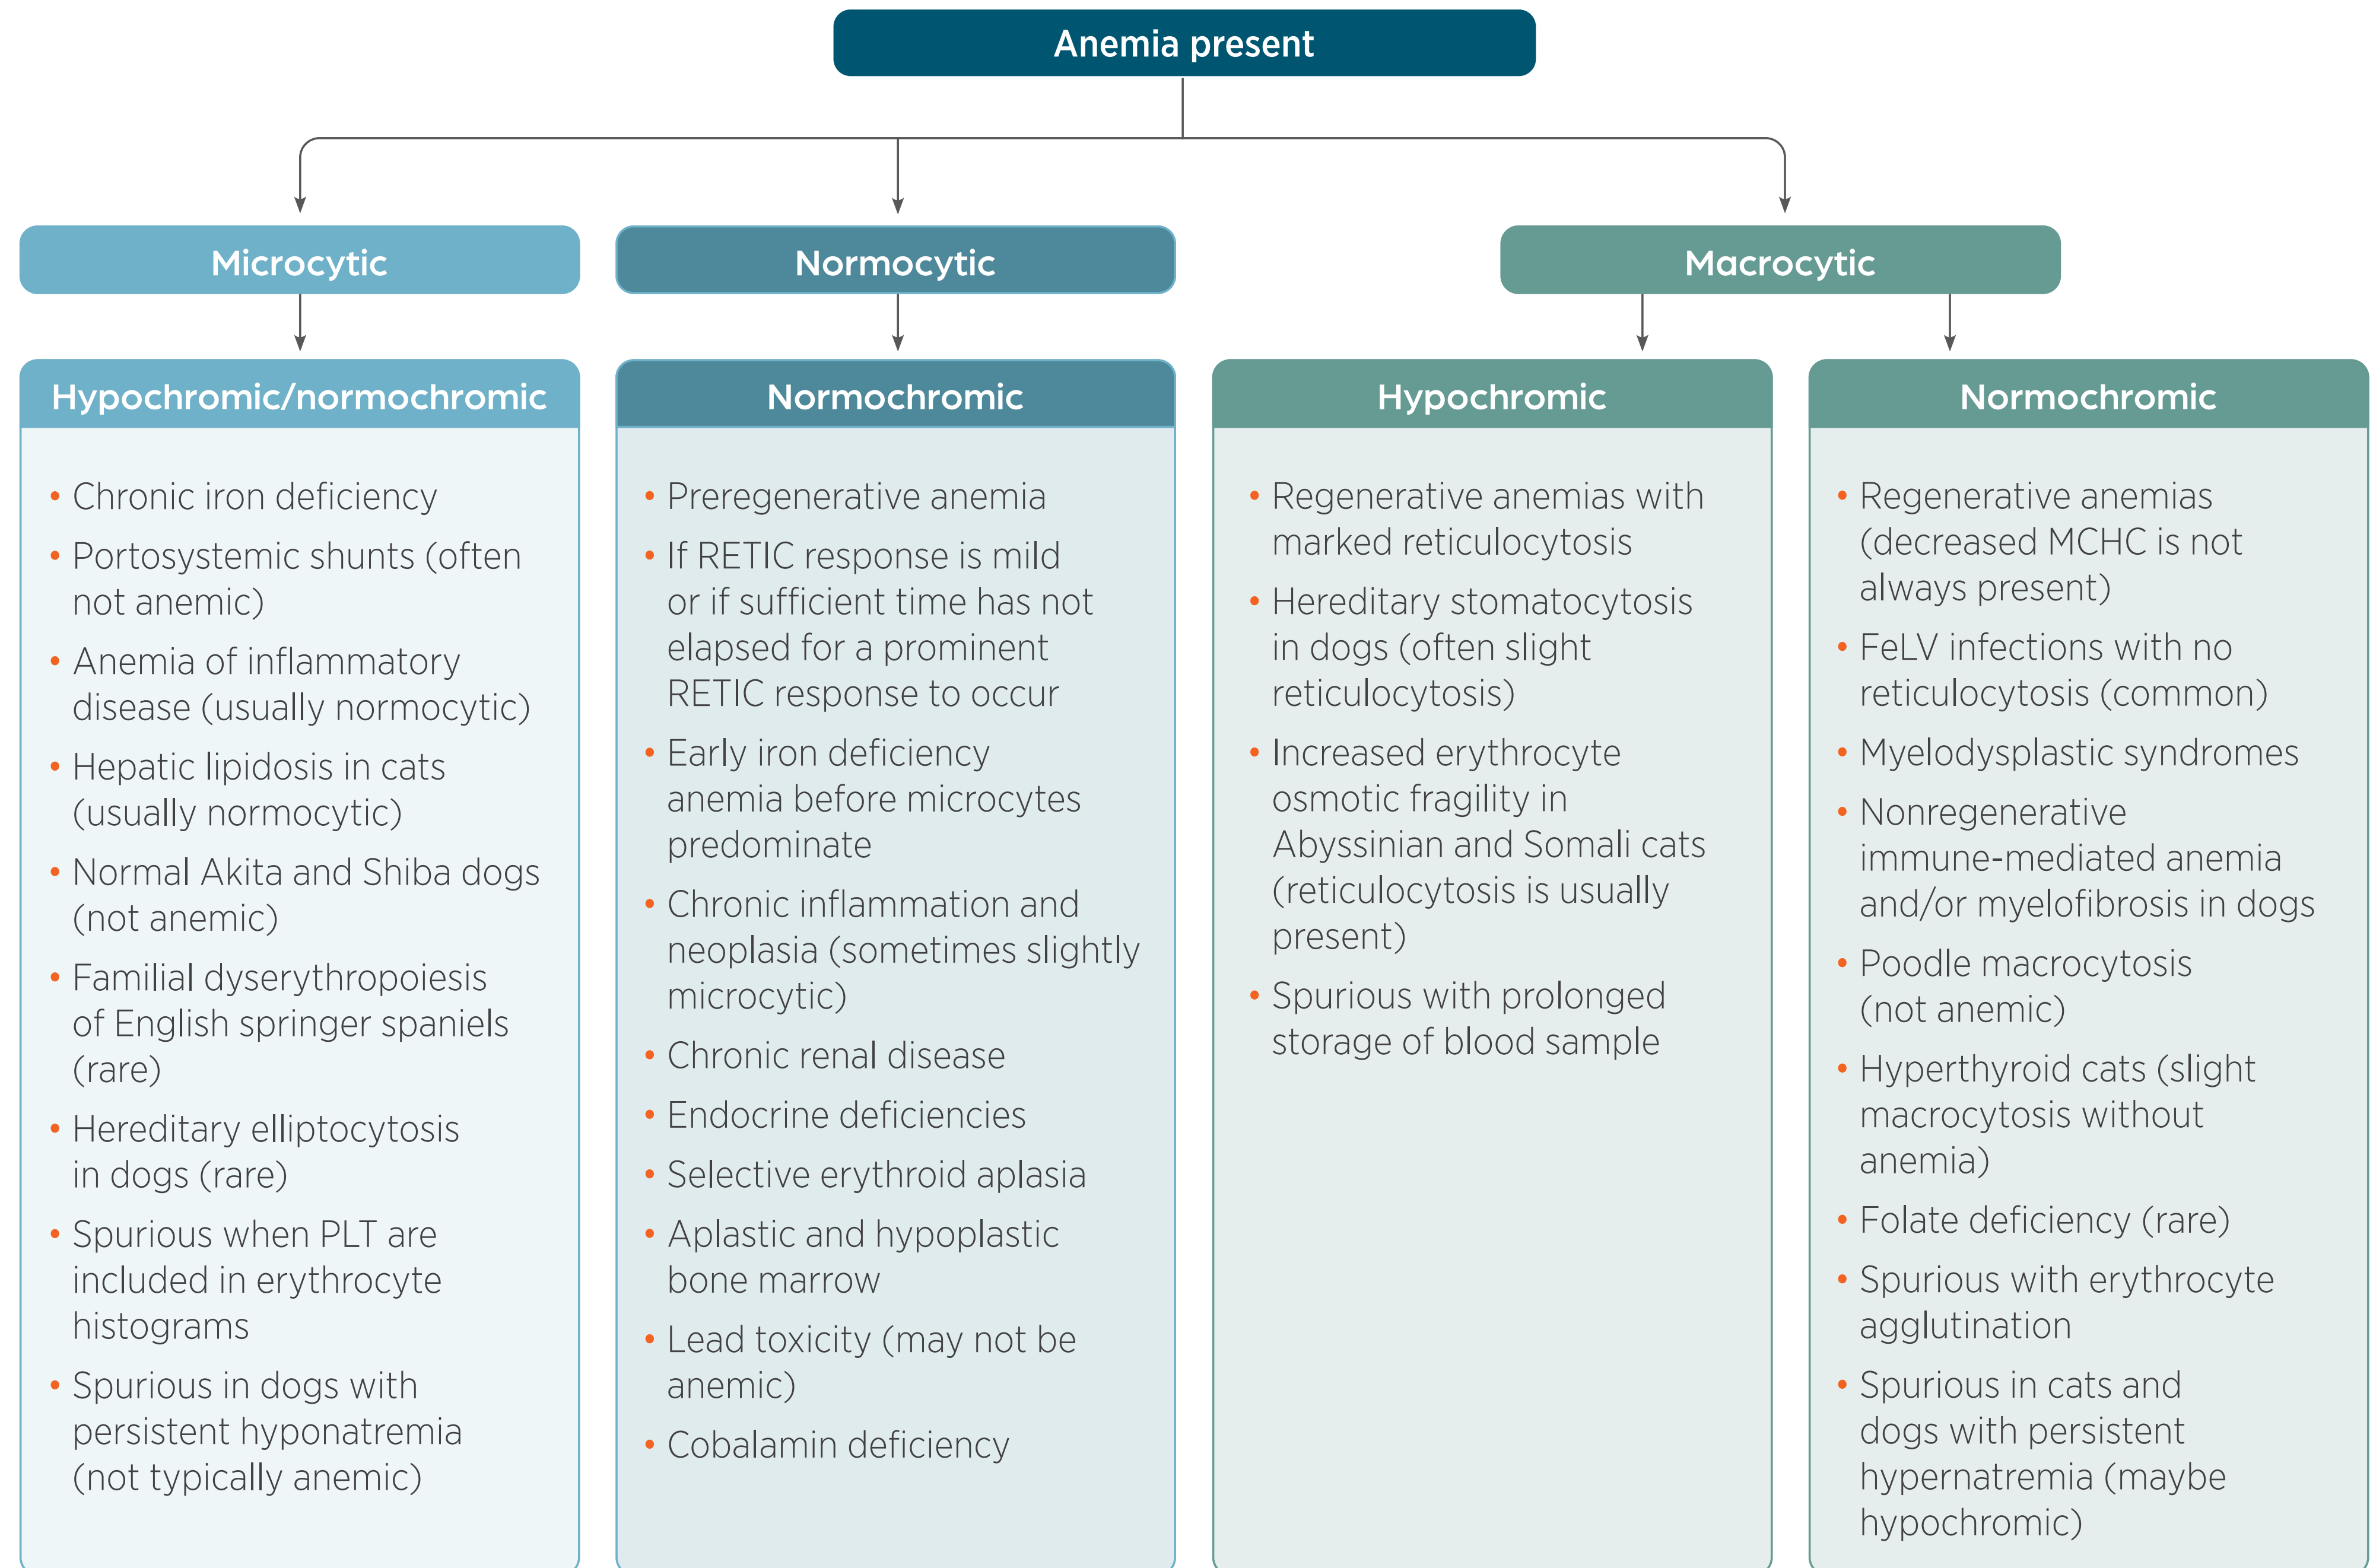

How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns

Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)



Alternative Fluids



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide


- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

Running alternative fluids on the VETSCAN HM5

Identify in-clinic nucleated cell counts* in alternative fluids (including pleural, peritoneal and synovial fluids) with the VETSCAN HM5. Characterize exudate samples to diagnose and identify potential inflammation, infections and neoplasia.

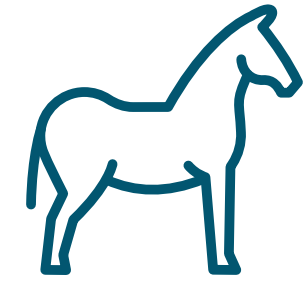

Validated for synovial fluid in horses^{36†}

Synovial fluid procedure

1. Add a flake of hyaluronidase[‡] (enzyme concentrate) to sample in a serum top tube, mix and store at room temperature for 10 minutes
2. Run the undiluted sample under the appropriate species setting on the VETSCAN HM5
3. Observe the total WBC number, which is useful in the determination of whether the WBC count is normal or abnormal
4. Microscopically evaluate a stained smear for a leukocyte differential and identification of nonleukocyte cells and/or infectious organisms
5. Perform a Soak Cleaning cycle (blue HM5) using HemaClean after every synovial fluid sample run



Validated for pleural and peritoneal fluid in dogs^{36†}

Pleural and peritoneal fluid procedure

1. Run undiluted sample in a serum tube under the appropriate species setting on the VETSCAN HM5
2. Observe the total WBC number, which is useful for classification of fluids and provides the total nucleated cell count
3. Perform a total protein concentration on a refractometer
4. Microscopically evaluate a stained smear for a leukocyte differential and identification of nonleukocyte cells and/or infectious organisms

Contact Diagnostic Technical Support 24/7 for assistance with interpreting VETSCAN HM5 troubleshooting reports



(888) 963-8471 (option 5)



dxsupport@zoetis.com

*VETSCAN HM5 analyzers are not intended to provide accurate differential cell counts for alternative fluid analysis samples.

†For results for species and/or fluids not validated, fluid samples may be run. However, precision and accuracy are not available, and results will not be supported by Zoetis Diagnostics.

‡Hyaluronidase from Sigma Chem Co, Part No. H3506, 100 mg bottle.

Reference Intervals (Ranges)



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples







Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

VETSCAN HM5 reference intervals, SI units⁷

Parameter	Units	 DOG	 CAT ³⁷	 HORSE	 CATTLE	 SHEEP*	 GOAT*
WBC	10 ⁹ cells/l	6.0 - 17.0	3.5 - 20.7	5.4 - 14.3	4.0 - 12.0	4.0 - 12.0	4.0 - 13.0
LYM	10 ⁹ cells/l	1.00 - 4.80	0.83 - 9.10	1.50 - 7.70	2.50 - 7.50	2.00 - 9.00	2.00 - 9.00
MON	10 ⁹ cells/l	0.20 - 1.50	0.09 - 1.21	0 - 1.50	0 - 0.84	0 - 0.75	0 - 0.50
NEU (GRA)	10 ⁹ cells/l	3.00 - 12.00	1.63 - 13.37	2.30 - 9.50	0.60 - 6.70	(0.70 - 7.30)	(1.20 - 8.00)
EOS	10 ⁹ cells/l	0 - 0.80	0.02 - 0.49	0 - 1.00	0.10 - 1.00	---	---
RBC	10 ¹² cells/l	5.5 - 8.5	7.7 - 12.8	6.8 - 12.9	5.0 - 10.0	9.0 - 15.8	5.5 - 8.5
HCT	%	37.0 - 55.0	33.7 - 55.4	32.0 - 53.0	24.0 - 46.0	27.0 - 45.0	37.0 - 55.0
HGB	g/l	120 - 180	100 - 170	110 - 190	80 - 150	90 - 150	120 - 180
MCV	fL	60 - 77	35 - 52	37 - 59	40 - 60	28 - 40	60 - 77
MCH	pg	19.5 - 24.5	10.0 - 16.9	12.3 - 19.7	11.0 - 17.0	8.0 - 12.0	19.5 - 24.5
MCHC	g/l	310 - 390	270 - 350	310 - 390	300 - 360	310 - 340	310 - 340
RDWc	%	14.0 - 20.0	18.3 - 24.1	N/A	N/A	N/A	N/A
PLT	10 ⁹ cells/l	165 - 500	125 - 618	100 - 400	100 - 800	100 - 800	200 - 500
MPV	fL	3.9 - 11.1	8.6 - 14.9	N/A	N/A	N/A	N/A

Reference intervals are determined from a population of healthy adult animals of a given species for a given test.

VETSCAN HM5 reference intervals continue on the next page.

---: EOS not included in 3-part differential.

N/A: Reference interval data not available for these parameters

*3-part differential with GRA.

Reference Intervals (Ranges)



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples









Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

VETSCAN HM5 reference intervals, SI units⁷ (cont'd)

Parameter	Units	 RABBIT*	 FERRET*	 GUINEA PIG*	 RAT*	 MOUSE**	 PIG*	 ALPACA	 LLAMA
WBC	10 ⁹ cells/l	3.0 - 11.5	2.0 - 10.0	5.0 - 17.0	2.1 - 19.5	6.0 - 15.0	11.0 - 22.0	6.0 - 30.0	8.0 - 23
LYM	10 ⁹ cells/l	2.00 - 9.10	0.40 - 6.50	2.00 - 15.00	2.00 - 14.10	3.40 - 7.44	5.50 - 11.10	1.00 - 20.00	1.00 - 6.00
MON	10 ⁹ cells/l	0 - 0.50	0.10 - 0.70	N/A	0 - 0.98	0 - 0.60	0.66 - 1.32	N/A	N/A
NEU (GRA)	10 ⁹ cells/l	(0 - 2.80)	(0.80 - 4.50)	(1.00 - 11.00)	(0.10 - 5.40)	(0.50 - 3.80)	(5.00 - 10.00)	3.00 - 20.00	5.00 - 24.00
EOS	10 ⁹ cells/l	---	---	---	---	---	---	N/A	N/A
RBC	10 ¹² cells/l	5.0 - 9.0	7.8 - 13.0	4.8 - 6.3	5.3 - 10.0	7.0 - 12.0	5.0 - 8.0	8.0 - 20.0	10.0 - 17.0
HCT	%	36.0 - 50.0	36.0 - 56.0	30.0 - 44.0	35.0 - 52.0	35.0 - 45.0	32.0 - 50.0	25.0 - 45.0	25.0 - 50.0
HGB	g/l	130 - 160	120 - 180	80 - 150	140 - 180	120 - 160	100 - 160	90 - 210	110 - 180
MCV	fL	57 - 70	40 - 48	50 - 90	50 - 62	45 - 55	50 - 68	15 - 35	20 - 35
MCH	pg	17.5 - 23.5	13.5 - 16.5	12.0 - 13.0	16.0 - 23.0	11.1 - 12.7	17.0 - 21.0	7.5 - 13.5	10.0 - 14.0
MCHC	g/l	300 - 380	320 - 350	300 - 360	310 - 400	220 - 320	300 - 340	300 - 450	300 - 450
RDWc	%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A
PLT	10 ⁹ cells/l	218 - 641	96 - 776	200 - 600	500 - 1000	200 - 450	325 - 715	N/A	N/A
MPV	fL	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A

VETSCAN HM5 reference intervals continue on the next page.

---: EOS not included in 3-part differential.

N/A: Reference interval data not available for these parameters

*3-part differential with GRA.

†Different mouse models may have varied intervals, and these reference intervals should be used only as a guideline.

Reference Intervals (Ranges)



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples







Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

VETSCAN HM5 reference intervals, common units⁷

Parameter	Units	 DOG	 CAT ³⁷	 HORSE	 CATTLE	 SHEEP*	 GOAT*
WBC	10 ⁹ cells/l	6.0 - 17.0	3.5 - 20.7	5.4 - 14.3	4.0 - 12.0	4.0 - 12.0	4.0 - 13.0
LYM	10 ⁹ cells/l	1.00 - 4.80	0.83 - 9.10	1.50 - 7.70	2.50 - 7.50	2.00 - 9.00	2.00 - 9.00
MON	10 ⁹ cells/l	0.20 - 1.50	0.09 - 1.21	0 - 1.50	0 - 0.84	0 - 0.75	0 - 0.50
NEU (GRA)	10 ⁹ cells/l	3.00 - 12.00	1.63 - 13.37	2.30 - 9.50	0.60 - 6.70	(0.70 - 7.30)	(1.20 - 8.00)
EOS	10 ⁹ cells/l	0 - 0.80	0.02 - 0.49	0 - 1.00	0.10 - 1.00	---	---
RBC	10 ¹² cells/l	5.5 - 8.5	7.7 - 12.8	6.8 - 12.9	5.0 - 10.0	9.0 - 15.8	5.5 - 8.5
HCT	%	37.0 - 55.0	33.7 - 55.4	32.0 - 53.0	24.0 - 46.0	27.0 - 45.0	37.0 - 55.0
HGB	g/dl	12 - 18	10 - 17	11 - 19	8 - 15	9 - 15	12 - 18
MCV	fL	60 - 77	35 - 52	37 - 59	40 - 60	28 - 40	60 - 77
MCH	pg	19.5 - 24.5	10.0 - 16.9	12.3 - 19.7	11.0 - 17.0	8.0 - 12.0	19.5 - 24.5
MCHC	g/dl	31 - 39	27 - 35	31 - 39	30 - 36	31 - 34	31 - 34
RDWc	%	14.0 - 20.0	18.3 - 24.1	N/A	N/A	N/A	N/A
PLT	10 ⁹ cells/l	165 - 500	125 - 618	100 - 400	100 - 800	100 - 800	200 - 500
MPV	fL	3.9 - 11.1	8.6 - 14.9	N/A	N/A	N/A	N/A

Reference intervals are determined from a population of healthy adult animals of a given species for a given test.

VETSCAN HM5 reference intervals continue on the next page.

---: EOS not included in 3-part differential.
 N/A: Reference interval data not available for these parameters
 *3-part differential with GRA.

Reference Intervals (Ranges)



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV/TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples









Interpretation Guide

- Macrothrombocytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

VETSCAN HM5 reference intervals, common units⁷ (cont'd)

Parameter	Units	 RABBIT*	 FERRET*	 GUINEA PIG*	 RAT*	 MOUSE**	 PIG*	 ALPACA	 LLAMA
WBC	10 ⁹ cells/l	3.0 - 11.5	2.0 - 10.0	5.0 - 17.0	2.1 - 19.5	6.0 - 15.0	11.0 - 22.0	6.0 - 30.0	8.0 - 23
LYM	10 ⁹ cells/l	2.00 - 9.10	0.40 - 6.50	2.00 - 15.00	2.00 - 14.10	3.40 - 7.44	5.50 - 11.10	1.00 - 20.00	1.00 - 6.00
MON	10 ⁹ cells/l	0 - 0.50	0.10 - 0.70	N/A	0 - 0.98	0 - 0.60	0.66 - 1.32	N/A	N/A
NEU (GRA)	10 ⁹ cells/l	(0 - 2.80)	(0.80 - 4.50)	(1.00 - 11.00)	(0.10 - 5.40)	(0.50 - 3.80)	(5.00 - 10.00)	3.00 - 20.00	5.00 - 24.00
EOS	10 ⁹ cells/l	---	---	---	---	---	---	N/A	N/A
RBC	10 ¹² cells/l	5.0 - 9.0	7.8 - 13.0	4.8 - 6.3	5.3 - 10.0	7.0 - 12.0	5.0 - 8.0	8.0 - 20.0	10.0 - 17.0
HCT	%	36.0 - 50.0	36.0 - 56.0	30.0 - 44.0	35.0 - 52.0	35.0 - 45.0	32.0 - 50.0	25.0 - 45.0	25.0 - 50.0
HGB	g/dl	13 - 16	12 - 18	8 - 15	14 - 18	12 - 16	10 - 16	9 - 21	11 - 18
MCV	fL	57 - 70	40 - 48	50 - 90	50 - 62	45 - 55	50 - 68	15 - 35	20 - 35
MCH	pg	17.5 - 23.5	13.5 - 16.5	12.0 - 13.0	16.0 - 23.0	11.1 - 12.7	17.0 - 21.0	7.5 - 13.5	10.0 - 14.0
MCHC	g/dl	30 - 38	32 - 35	30 - 36	31 - 40	22 - 32	30 - 34	30 - 45	30 - 45
RDWc	%	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A
PLT	10 ⁹ cells/l	218 - 641	96 - 776	200 - 600	500 - 1000	200 - 450	325 - 715	N/A	N/A
MPV	fL	N/A	N/A	N/A	N/A	N/A	N/A	N/A	N/A

Need help? Contact Diagnostic Technical Support 24/7

 (888) 963-8471 (option 5)  dxsupport@zoetis.com

---: EOS not included in 3-part differential.

N/A: Reference interval data not available for these parameters

*3-part differential with GRA.

†Different mouse models may have varied intervals, and these reference intervals should be used only as a guideline.



References



How VETSCAN® HM5 Works

Sample Handling

- Patient preparation
- Sample collection
- Running a sample

Complete Hematology Picture

- Minimum database
- Automated CBC
- Blood smear
- PCV / TS

Responsible Patient Trending

Histograms

- Interpreting histograms
- Histogram examples

Interpretation Guide

- Macrothrombo-cytopenia
- Leukogram patterns
- Understanding anemia

Alternative Fluids

Reference Intervals (Ranges)

References: 1. Bürgi W, Marti HR. Automated blood count analysis by trimodal size distribution of leukocytes with the SYSMEX E-5000. *J Clin Chem Clin Biochem.* 1989;27(6):365-368. doi:10.1515/cclm.1989.27.6.365. 2. Münster M. Overview of the benefits of switching from a 3-part differential to a 5-part differential haematology analyser. March 2012. Accessed May 31, 2022. <https://www.sysmex-europe.com/academy/library/documents/detail/seed-overview-of-the-benefits-of-switching-from-a-3-part-differential-to-a-5-part-differential-haematology-analyser.html>. 3. Monti P, Archer J. Quality assurance and interpretation of laboratory data. In: Villiers E, Ristic J, eds. *BSAVA Manual of Canine and Feline Clinical Pathology*. 3rd ed. British Small Animal Veterinary Association; 2016:11-26. 4. Sample collection. Cornell University College of Veterinary Medicine. Accessed August 3, 2022. <https://eclinpath.com/hematology/sample-collection-heme/>. 5. Weiss DJ. Drug-associated blood cell dyscrasias. *Compend Contin Educ Vet.* 2012;34(6):E2. 6. Allison RW. Laboratory evaluation of the pancreas and glucose metabolism. In: Thrall MA, Weiser G, Allison RW, et al, eds. *Veterinary Hematology and Clinical Chemistry*. 2nd ed. Wiley-Blackwell; 2012:425-440. 7. Data on file, VETSCAN HM5 Operator's Manual, 2018, Zoetis Inc. 8. Villiers E. Introduction to haematology. In: Villiers E, Ristic J, eds. *BSAVA Manual of Canine and Feline Clinical Pathology*. 3rd ed. British Small Animal Veterinary Association; 2016:27-37. 9. Villiers E. Disorders of erythrocytes. In: Villiers E, Ristic J, eds. *BSAVA Manual of Canine and Feline Clinical Pathology*. 3rd ed. British Small Animal Veterinary Association; 2016:38-66. 10. Kipperman BS. The demise of the minimum database. *J Am Vet Med Assoc.* 2014;244(12):1368-1370. doi:10.2460/javma.244.12.1368. 11. Zabolotzky SM, Walker DB. Peripheral blood smears. In: Cowell RL, Valenciano AC, eds. *Cowell and Tyler's Diagnostic Cytology and Hematology of the Dog and Cat*. 5th ed. Elsevier Inc.; 2019:438-467. 12. Weiss DJ, Tvedten H. The complete blood count, bone marrow examination, and blood banking: general comments and selected techniques. In: Willard MD, Tvedten H, eds. *Small Animal Clinical Diagnosis by Laboratory Methods*. 5th ed. Elsevier Inc.; 2012:12-37. 13. Stirn M, Moritz A, Bauer N. Rate of manual leukocyte differentials in dog, cat and horse blood samples using ADVIA 120 cytograms. *BMC Vet Res.* 2014;10:125. doi:10.1186/1746-6148-10-125. 14. Sharkey L, Heinrich D. In-clinic hematology: the blood film review. *Today's Veterinary Practice.* 2015. Accessed January 5, 2022. <https://todaysveterinarypractice.com/in-clinic-hematology-the-blood-film-review/>. 15. Harvey JW. Hematology procedures. In: Harvey JW, ed. *Veterinary Hematology: A Diagnostic Guide and Color Atlas*. 1st ed. Elsevier Inc.; 2012:11-32. 16. Brockus CW. Erythrocytes. In: Latimer KS, Mahaffey EA, Prasse KW, eds. *Duncan & Prasse's Veterinary Laboratory Medicine: Clinical Pathology*. 4th ed. Wiley-Blackwell; 2003:3-15. 17. Weiser G. Laboratory technology for veterinary medicine. In: Thrall MA, Weiser G, Allison RW, et al, eds. *Veterinary Hematology and Clinical Chemistry*. 2nd ed. Wiley-Blackwell; 2012:3-33. 18. Stockham SL, Scott MA. Erythrocytes. In: Stockham SL, Scott MA, eds. *Fundamentals of Veterinary Clinical Pathology*. 2nd ed. Wiley-Blackwell; 2008:110-221. 19. Erythrogram. Cornell University College of Veterinary Medicine. Accessed July 27, 2022. <https://eclinpath.com/hematology/hemogram-basics/erythrogram/>. 20. Walton RM. Subject-based reference values: biological variation, individuality, and reference change values. *Vet Clin Pathol.* 2012;41(2):175-181. doi:10.1111/j.1939-165X.2012.00414.x. 21. Ralston SL. Care for the older horse: diet and health. Equine Science Center. Published 2004. Accessed October 10, 2022. https://esc.rutgers.edu/fact_sheet/care-for-the-older-horse-diet-and-health/. 22. Thomas ET, Bhagya S, Majeed A. Clinical utility of blood cell histogram interpretation. *J Clin Diagn Res.* 2017;11(9):OE01-OE04. doi:10.7860/JCDR/2017/28508.10620. 23. Athanasiou LV, Tsokana CN, Pardali D, et al. Histograms of complete blood counts in dogs: maximizing diagnostic information. *Top Companion Anim Med.* 2018;33(4):141-146. doi:10.1053/j.tcam.2018.06.001. 24. HM5: Interpreting histograms handout sheet. Data on file, ABX-00198, 2019, Zoetis Inc. 25. Constantino BT. The red cell histogram and the dimorphic red cell population. *Laboratory Medicine.* 2011;42(5):300-308. 26. Data on file, Study No. TI-04205, 2012, Zoetis Inc. 27. Stokol T. Disorders of haemostasis. In: Villiers E, Ristic J, eds. *BSAVA Manual of Canine and Feline Clinical Pathology*. 3rd ed. British Small Animal Veterinary Association; 2016:94-122. 28. Data on file, Study No. TI-04255, Zoetis Inc. 29. Data on file, Study No. TI-04614, 2012, Zoetis Inc. 30. Breznock EM, Strack D. Effects of the spleen, epinephrine, and splenectomy on determination of blood volume in cats. *Am J Vet Res.* 1982;43(11):2062-2066. 31. Allard RL, Carlos AD, Faltin EC. Canine hematologic changes during gestation and lactation. *Compan Anim Pract.* 1989;19(3):3-6. 32. Berman E. Hemogram of the cat during pregnancy and lactation and after lactation. *Am J Vet Res.* 1974;35(3):457-460. 33. Grimes CN. Laboratory diagnosis and classification of anemia. Presented at: ACVIM Forum; June 9-11, 2016; Denver, Colorado. 34. Data on file, FUNDamentals of Hematology: Diagnosing Anemia, Zoetis Inc. 35. Data on file, TI-08180, 2022, Zoetis Inc. 36. Brudvig JM, Swenson CL. Total nucleated cell and leukocyte differential counts in canine pleural and peritoneal fluid and equine synovial fluid samples: comparison of automated and manual methods. *Vet Clin Pathol.* 2015;44(4):570-579. doi:10.1111/vcp.12298. 37. Data on file, Study No. DH86R-US-20-058, Zoetis Inc.